



Integra®
Forefoot
Mid & HindFoot
Large Bones
Products Catalogue

Table of Contents

Warranty Information	5
Integra® Forefoot Solutions	7
Forefoot Set	8
Bold® Compression Screw dia. 2.5 mm / 3.0 mm / 3.7 mm	14
QWIX® Fixation Screw dia. 3.0 mm	14
SPIN® Screw dia. 2.0 mm / 2.7 mm	15
UNI-CLIP® Compressive Staple	16
SOLUSTAPLE® Standard Staple	16
Osteoguides	17
K-FIX® - K-wire End Protector	17
Weil Clamp	17
B-BOP® LOCK plate	18
IPP-ON® Interphalangeal Arthrodesis Implant	19
METIS® Metatarso-phalangeal prosthesis	20
K2™ Hemi Toe Implant	22
Movement Great Toe system	23
HALLU®-FIX MTP Arthrodesis System	24
HALLU® Plates	24
HALLU® SNAP-OFF® Screws	25
HALLU®-FIX Instruments	25
HALLU®-LOCK Arthrodesis System	26
HALLU®-REAM set	28
DPR System Minimal Invasive Foot Surgery	29
Post-Operative Shoes	30
Integra® Mid & HindFoot Solutions	33
Subtalar Arthrodesis	34
QWIX® Fixation screw	34
Large QWIX® Fixation and Positioning Screws	35
I.C.O.S.® Ideal Compression Screw	36
Flatfoot implants	39
KALIX® II Flat Foot Implant	39
MBA™ Titanium Subtalar Implant	40

Dorsal Lisfranc plate & Medial Lisfranc plate	41
ADVANSYS [®] Lisfranc Plate	41
UNI-CP [™] Compression Plate	43
Ankle Solutions	44
Total Ankle Replacement Hintegra [®] prosthesis	44
Ankle Fusion	54
PANTA [®] Nail	54
ADVANSYS [®] Plate	59
TIBIAXYS [®] Plating System	61
Minimally Invasive Achilles Tendon Ruptures	64
ACHILLON [®] System	64
Surgical Instruments	65
Hintermann [®] Distractors	65
Osteoguides	66
K-FIX [®] Protector	66
Weil Clamp	66
General Optional Instruments	67
Post-Operatives Shoes	68
Surfix[®] osteotomy solutions	70
Knee osteotomy plates	72
POF plate	72
PTO plate	73
POM plate	74
PTC plate	75
PTF plate	76
ATAO [®] Bone Graft Substitute	77
Set osteotomy	77
Pediatric osteotomy plates	78
PSFE plates	78
PDTL plates	80
Pediatric set	82
Product References	85

Pricing:

Prices stated in specific written quotations are firm for thirty days from the date given, and are otherwise subject to change without prior notice. Pricing terms stated on written agreements are governed by such agreements.

Minimum Order Requirements:

Minimum order requirement is €250 (a €20 minimum order requirement charge will be added to any order under €250).

Ordering Procedure:

A written purchase order on the customer's form may be requested for purchases of Integra LifeSciences products.

Acceptance of Orders:

Orders are accepted upon approval by Integra Customer Service.

Return Policy:

- Authorization from Customer Service must be obtained prior to returning product.
- Sterile product must be returned in unopened, undamaged cartons, packed to prevent damage.
- Non-sterile product must be returned in unused saleable condition in original package.
- Custom or special order products will not be accepted for credit.
- Credit will be issued for goods returned prior to ninety days from ship date with a 20% restocking charge. This assumes that the product returned is not damaged and can be verified to have not been used or opened.

Integra Limited Warranty – Integra products

INTEGRA LIFESCIENCES CORPORATION and its wholly owned subsidiaries ("INTEGRA") warrant to INTEGRA authorized distributors and the original purchaser only that each new INTEGRA Surfix® product is free from manufacturing defects in material and workmanship when used for its intended surgical purpose. For purposes of products sold by INTEGRA through an authorized distributor of INTEGRA, "original purchaser" shall include the purchaser of INTEGRA products to whom the distributor first sells the product.

If any covered defect occurs, the purchaser or distributor should communicate directly with INTEGRA. If purchaser or distributor seeks to invoke the terms of this warranty, the product must be returned to INTEGRA. The defective product should be returned promptly, properly packaged and postage prepaid. Loss or damage in return shipment to INTEGRA shall be at sender's risk. INTEGRA's sole responsibility under this warranty shall be repair or replacement, at INTEGRA's sole discretion at INTEGRA's expense, subject to the terms of this warranty and applicable agreements.

INTEGRA provides for no commercial or additional warranty whatsoever, except as may be otherwise expressly agreed in a separate commercial agreement or undertaking duly signed by an INTEGRA authorised representative.

IN NO EVENT SHALL INTEGRA BE LIABLE FOR ANY INCIDENTAL, INDIRECT, CONSEQUENTIAL OR PUNITIVE DAMAGES IN CONNECTION WITH THE ACQUISITION OR USE OF ANY INTEGRA PRODUCT. Further, this warranty shall not apply to, and INTEGRA shall not be responsible for, any loss arising in connection with the purchase or use of any INTEGRA product that has been repaired by anyone other than an authorized INTEGRA service representative or altered in any way so as, in INTEGRA's judgment, to affect its stability or reliability, or which has been subject to misuse, negligence or accident, or which has been used otherwise than in accordance with the instructions furnished by INTEGRA.

Customer Service Contact Information:**International**

+33 (0)4 37 47 59 50

+33 (0)4 37 47 59 25 (Fax)

csemea@Integralife.com

Benelux

+32 (0)2 257 4130

+32 (0)2 253 2466 (Fax)

custsvcbenelux@Integralife.com

France

+33 (0)4 37 47 59 10

+33 (0)4 37 47 59 29 (Fax)

cs-ortho@Integralife.com

Switzerland

+41 (0)2 27 21 23 30

+41 (0)2 27 21 23 99 (Fax)

custsvcsuisse@Integralife.com

United Kingdom

+44 (0)1 264 345 780

+44 (0)1 264 363 782 (Fax)

custsvcs.uk@integralife.com

THIS INTEGRA LIMITED WARRANTY IS EXCLUSIVE AND IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, AND OF ALL OTHER OBLIGATIONS OR LIABILITIES ON INTEGRA'S PART OR THE PART OF ITS DISTRIBUTORS, AND INTEGRA NEITHER ASSUMES NOR AUTHORIZES ANY REPRESENTATIVE OR OTHER PERSON TO ASSUME FOR IT ANY OTHER LIABILITY IN CONNECTION WITH INTEGRA'S PRODUCTS.

INTEGRA DISCLAIMS ALL OTHER WARRANTIES, EXPRESS OR IMPLIED INCLUDING ANY IMPLIED WARRANTY OF MERCHANTABILITY OR OF FITNESS FOR A PARTICULAR PURPOSE OR APPLICATION OR WARRANTY OF QUALITY AS WELL AS ANY EXPRESS OR IMPLIED WARRANTY TO PATIENTS. No warranty or guarantee may be created by any act or statement nor may this Standard Warranty be modified in any way, except as a result of a writing signed by an officer of INTEGRA. These limitations on the creation or modification of this warranty may not be waived or modified orally or by any conduct.

IN NO EVENT SHALL INTEGRA AUTHORIZED DISTRIBUTORS BE LIABLE TOWARDS THE ORIGINAL PURCHASER FOR ANY INCIDENTAL, INDIRECT, CONSEQUENTIAL OR PUNITIVE DAMAGES IN CONNECTION WITH THE ACQUISITION OR USE OF ANY INTEGRA PRODUCT. Further, this warranty shall not apply to, and INTEGRA authorized distributors shall not be responsible towards the original purchaser for, any loss, arising in connection with the purchase or use of any INTEGRA product that has been repaired by anyone other than an authorized INTEGRA service representative or altered in any way so as to affect its stability or reliability, or which has been subject to misuse, negligence or accident, or which has been used otherwise than in accordance with the instructions furnished by INTEGRA. THIS INTEGRA DISTRIBUTOR LIMITED WARRANTY IS EXCLUSIVE AND IN LIEU OF ALL OTHER WARRANTIES TOWARDS THE ORIGINAL PURCHASER, EXPRESS OR IMPLIED, AND OF ALL OTHER OBLIGATIONS OR LIABILITIES TOWARDS THE ORIGINAL PURCHASER ON INTEGRA AUTHORIZED DISTRIBUTOR'S PART.

INTEGRA AUTHORIZED DISTRIBUTORS DISCLAIM ALL OTHER WARRANTIES TOWARDS THE ORIGINAL PURCHASER, EXPRESS OR IMPLIED INCLUDING ANY IMPLIED WARRANTY OF MERCHANTABILITY OR OF FITNESS FOR A PARTICULAR PURPOSE OR APPLICATION OR WARRANTY OF QUALITY AS WELL AS ANY EXPRESS OR IMPLIED WARRANTY TO PATIENTS.

All the references numbers mentioned on this document are CE marked according to European council directive 93/42/EEC on medical devices and its relatives, unless specifically identified as "NOT CE MARKED".

250
240
230
220
210
200
190
180
170
160
150
140
130
120
110
100
90
80
70
60
50
40
30
20
10
0
MILLIMETERS





Integra® Forefoot Solutions

Forefoot Set

A new modular and scalable forefoot instruments set:

- Bold[®] 2.5 – 3.0 – 3.7 Compression screw.
- QWIX[®] 3.0 Fixation screw.
- Spin[®] 2.0 – 2.7 Spin break off screws.
- Solustaple[®] Standard staple.
- Uni-clip[®] Compression Staple.

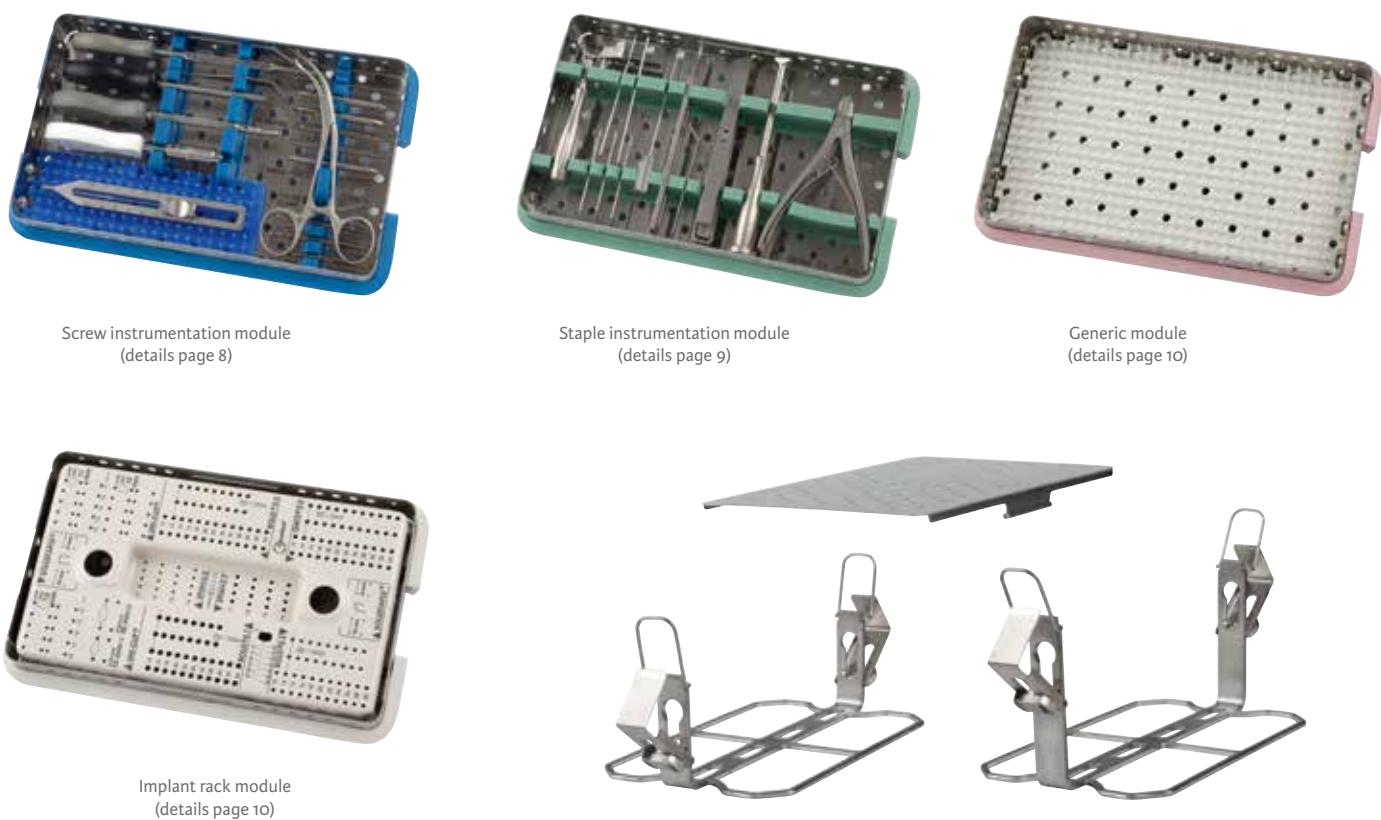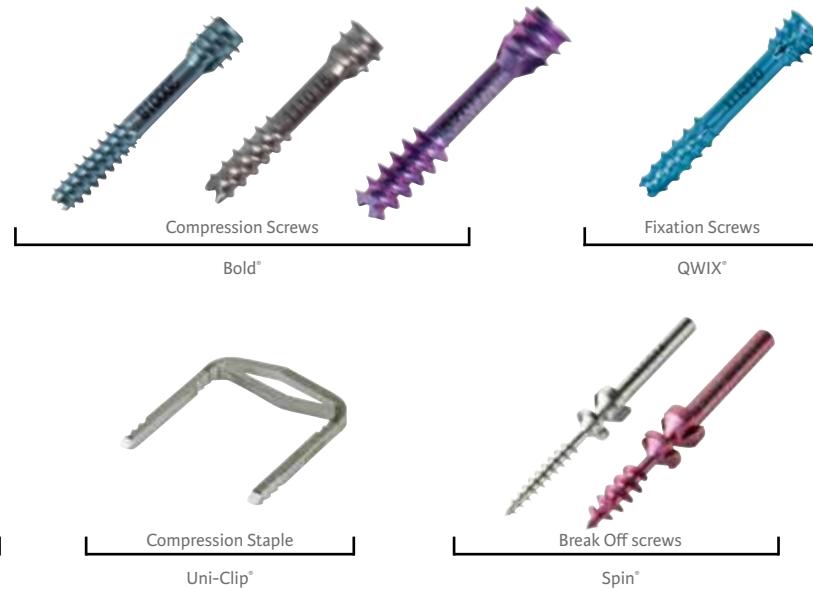

Frame

229996	Frame - 2 floors
229990	Frame - 3 floors
229970	Forefoot II- lid- generic



- Staple instrumentation
- Screw instrumentation




- Non sterile Implants
- Staple instrumentation
- Screw instrumentation



- Non sterile Implants
- Generic module
- Screw instrumentation

Forefoot Set – Screw Module

Reference	Description
119105	Scarf clamp
229002	Screwdriver - Hexa 2.0
229005	AO Screwdriver - Hexa 2.0 - AO Attachment - Cannulated
229003	Screwdriver - T7 Star - Cannulated
229004	Screwdriver - AO - T7 Star - Cannulated
997301	Depth Gauge
997311	AO Straight Handle
229011	Longitudinal Cutting Guide (Optional)
229012	Transversal Cutting Guide (Optional)
229101	Ruler
229951	Sterilization Screws Container including:
229961	Tray
229970	Lid
229971	Mat

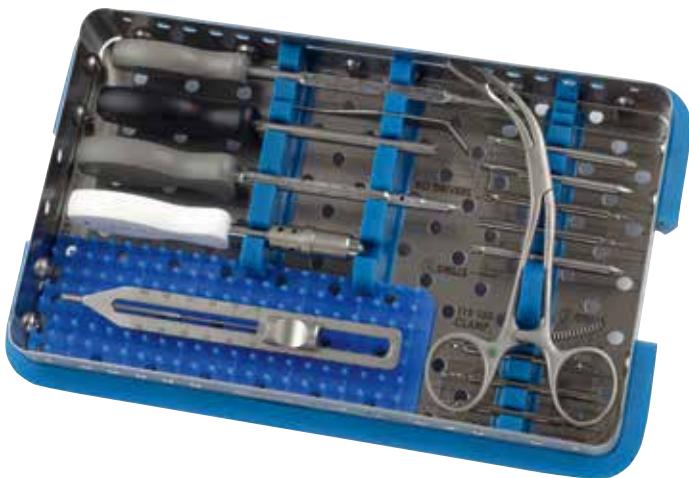

Drill Reference	Corresponding Product	2 in 1	Diameter	Cannulated	Length	AO attachment
159 027 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm	■	12 mm	■
159 025 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm	■	22 mm	■
159 023 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm	■	32 mm	■
119 227 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm		12 mm	
119 225 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm		22 mm	
119 223 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm		32 mm	
119 027 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm	■	12 mm	
119 025 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm	■	22 mm	
119 023 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm	■	32 mm	
159 227 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm		12 mm	■
159 225 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm		22 mm	■
159 223 (S)	Bold® 3.0 / Bold® 3.7	■	2.2 - 3.0 mm		32 mm	■
229 027 S	Bold® 2.5	■	1.9 - 2.5 mm	■	12 mm	■
229 037 S	Bold® 2.5	■	1.9 - 2.5 mm	■	22 mm	■
229 227 S	Bold® 2.5	■	1.9 - 2.5 mm	■	12 mm	
229 237 S	Bold® 2.5	■	1.9 - 2.5 mm	■	22 mm	
229 028 S	Bold® 2.5	■	1.9 - 2.5 mm		12 mm	■
229 038 S	Bold® 2.5	■	1.9 - 2.5 mm		22 mm	■
229 228 S	Bold® 2.5	■	1.9 - 2.5 mm		12 mm	
229 238 S	Bold® 2.5	■	1.9 - 2.5 mm		22 mm	

K-wire Reference	Corresponding Product	Diameter	Length
115 070 (S)	Bold® 3.0 / Bold® 3.7	1.0 mm	70 mm
115 100 (S)	Bold® 3.0 / Bold® 3.7	1.0 mm	100 mm
115 008 S	Bold® 2.5	0.8 mm	70 mm

All drills and K-wires are delivered sterile or non sterile except Bold® 2.5 K-wire which is only delivered in sterile.

(S) means available in sterile and non sterile

Forefoot Set – Staple Module

UNI-CLIP® Associated Instrument


229201	Uni-Clip® Drilling guide
229202	Uni-Clip® impactor
119311	Uni-Clip® spreading force

Solustaple® Associated Instrument

229102	Solustaple® impactor 90° & 26°
229101	Solustaple® drilling guide
997301	Depth gauge - dia 2.0 X L. 10 - 60 mm

Sterilization Container

229952 Staples container includes:
229962
229970

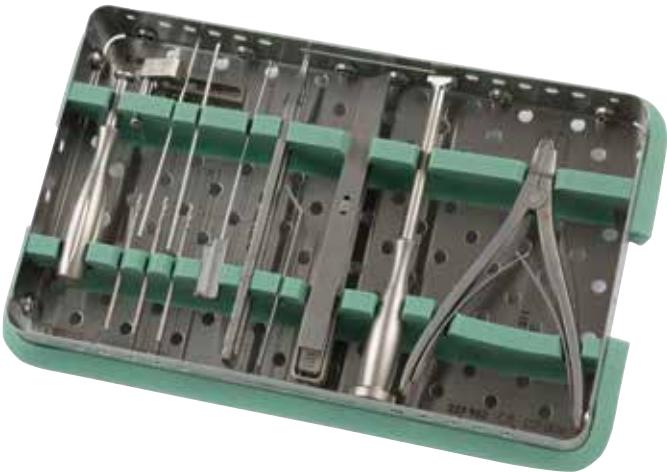

Drill Reference	Corresponding Product	Diameter	Cannulated	Length	AO attachment
119 004 (S)	Uni-Clip®	2.2 mm	■	34 mm	
119 006 (S)	Uni-Clip®	2.2 mm		34 mm	
159 004 (S)	Uni-Clip®	2.2 mm	■	34 mm	■
119 016 (S)	Uni-Clip®	2.2 mm		34 mm	■

K-wire Reference	Corresponding Product	Diameter	Length
115 070 (S)	Uni-Clip®	1.0 mm	70 mm
115 100 (S)	Uni-Clip®	1.0 mm	100 mm

All drills and K-wires are delivered sterile or non sterile except Bold® 2.5 K-wire which is only delivered in sterile.


(S) means available in sterile and non sterile

Forefoot Set – Implant Module

Sterilization Container

229965 Forefoot II - tray - non sterile implants

229975 Forefoot II - rack - non sterile implants

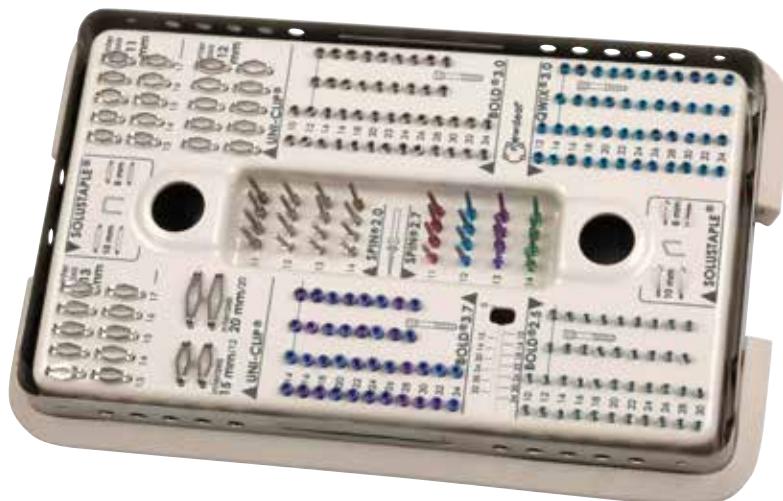

Forefoot Set – Generic Module

Sterilization Container

229966 Forefoot II - tray - generic

229976 Forefoot II - mat - generic



250
240
230
220
210
200
190
180
170
160
150
140
130
120
110
100
90
80
70
60
50
40
30
20
10
0
MILLIMETERS

Bold® Compression Screw Dia. 2.5 mm / 3.0 mm / 3.7 mm

(for associated instrumentation, see p. 8)

For fixation of bone fractures or for bone reconstruction.

- Totally intra-osseous implants.
- Large range of sizes:
 - > 10 to 30 mm for Bold® 2.5 screws by 2 mm increment.
 - > 10 to 34 mm for Bold® 3.0 screws by 2 mm increment.
 - > 14 to 34 mm for Bold® 3.7 screws by 2 mm increment.
- K-Wire guided drilling and insertion.
- Self tapping.
- True & controlled compression.
- Dual threads.
- Material: Titanium alloy TA6V.



Bold® dia 2.5 mm

Reference	Length
200010(S)	L. 10 mm
200012(S)	L. 12 mm
200014(S)	L. 14 mm
200016(S)	L. 16 mm
200018(S)	L. 18 mm
200020(S)	L. 20 mm
200022(S)	L. 22 mm
200024(S)	L. 24 mm
200026(S)	L. 26 mm
200028(S)	L. 28 mm
200030(S)	L. 30 mm

Bold® dia 3.0 mm

Reference	Length
111010(S)	L. 10 mm
111012(S)	L. 12 mm
111014(S)	L. 14 mm
111016(S)	L. 16 mm
111018(S)	L. 18 mm
111020(S)	L. 20 mm
111022(S)	L. 22 mm
111024(S)	L. 24 mm
111026(S)	L. 26 mm
111028(S)	L. 28 mm
111030(S)	L. 30 mm
111032(S)	L. 32 mm
111034(S)	L. 34 mm

Bold® dia 3.7 mm

Reference	Length
131014(S)	L. 14 mm
131016(S)	L. 16 mm
131018(S)	L. 18 mm
131020(S)	L. 20 mm
131022(S)	L. 22 mm
131024(S)	L. 24 mm
131026(S)	L. 26 mm
131028(S)	L. 28 mm
131030(S)	L. 30 mm
131032(S)	L. 32 mm
131034(S)	L. 34 mm

QWIX® Fixation Screw, Dia. 3.0 mm

(for associated instrumentation, see p. 8)

For fixation of bone fractures or for bone reconstruction.

- Self-drilling and self-tapping.
- Totally intra-osseous fixation.
- K-Wire guided drilling and insertion.
- Material: Titanium alloy TA6V.



QWIX® Dia. 3.0 mm

Reference	Length
111312(S)	L. 12 mm
111314(S)	L. 14 mm
111316(S)	L. 16 mm
111318(S)	L. 18 mm
111320(S)	L. 20 mm
111322(S)	L. 22 mm
111324(S)	L. 24 mm
111326(S)	L. 26 mm
111328(S)	L. 28 mm
111330(S)	L. 30 mm
111332(S)	L. 32 mm
111334(S)	L. 34 mm

(S) means available in sterile and non sterile

SPIN[®] Break Off Screw, Dia. 2.0 mm (for associated instrumentation, see p. 8)

For bone fixation.

- Break-off barrel.
- Self-drilling and self-tapping.
- Material: Titanium alloy TA6V.

Reference	Description
112011(S)	Spin [®] Dia. 2.0 x L. 11 mm
112012(S)	Spin [®] Dia. 2.0 x L. 12 mm
112013(S)	Spin [®] Dia. 2.0 x L. 13 mm
112014(S)	Spin [®] Dia. 2.0 x L. 14 mm


SPIN[®] Break Off Screw, Dia. 2.7 mm (for associated instrumentation, see p. 8)

Spin[®] 2.7 screw is recommended for soft or osteoporotic bones fixation.

- Break-off barrel.
- Self-drilling and self-tapping.
- Material: Titanium alloy TA6V.

Reference	Length
112111(S)	Spin [®] Dia. 2.7 x L. 11 mm
112112(S)	Spin [®] Dia. 2.7 x L. 12 mm
112113(S)	Spin [®] Dia. 2.7 x L. 13 mm
112114(S)	Spin [®] Dia. 2.7 x L. 14 mm



Color coded



(S) means available in sterile and non sterile

UNI-CLIP® Notched Staples

(for associated instrumentation, see p. 9)

For fixation of bone fractures or for bone reconstruction.

- Range sizes:
 - > Interaxis: 11, 12, 13, 15 and 20 mm.
 - > Leg lengths: 12, 13, 14, 15, 16, 17 and 20 mm.
- Material: Stainless steel 316L.



Reference	Description
213113(S)	Uni-Clip® interaxis 11.0 x L. 13 mm
213114(S)	Uni-Clip® interaxis 11.0 x L. 14 mm
213115(S)	Uni-Clip® interaxis 11.0 x L. 15 mm
213116(S)	Uni-Clip® interaxis 11.0 x L. 16 mm
213117(S)	Uni-Clip® interaxis 11.0 x L. 17 mm
213213(S)	Uni-Clip® interaxis 12.0 x L. 13 mm
213214(S)	Uni-Clip® interaxis 12.0 x L. 14 mm
213215(S)	Uni-Clip® interaxis 12.0 x L. 15 mm
213216(S)	Uni-Clip® interaxis 12.0 x L. 16 mm
213217(S)	Uni-Clip® interaxis 12.0 x L. 17 mm
213313(S)	Uni-Clip® interaxis 13.0 x L. 13 mm
213314(S)	Uni-Clip® interaxis 13.0 x L. 14 mm
213315(S)	Uni-Clip® interaxis 13.0 x L. 15 mm
213316(S)	Uni-Clip® interaxis 13.0 x L. 16 mm
213317(S)	Uni-Clip® interaxis 13.0 x L. 17 mm
213512(S)	Uni-Clip® interaxis 15.0 x L. 12 mm
213820(S)	Uni-Clip® interaxis 20.0 x L. 20 mm

SOLUSTAPLE® Standard Staple

(for associated instrumentation, see p. 9)

Static staple for fixation of mono cortical phalangeal osteotomies.

- Two shapes of staples (26° and 90°) are available.
- Self-perforating.
- Material: stainless steel 316L.



Reference	Description
114002(S)	Solustaple® 90° interaxis 8 mm
114004(S)	Solustaple® 90° interaxis 10 mm
114023(S)	Solustaple® 26° interaxis 8 mm
114025(S)	Solustaple® 26° interaxis 10 mm

(S) means available in sterile and non sterile

Osteoguides

- Suggested use:
 - > Scarf osteotomy.
 - > Chevron osteotomy.
 - > Basal osteotomy.
 - > Arthrodesis.
 - > Wedge osteotomies (Akin...).
- Details:
 - > Hole for K-Wire: Diameter 1.0 to 1.6 mm.
 - > Knurled handle for optimal grip.
 - > Blade thickness maxi 0.8 mm.
 - > Positioning tip.

Reference	Description
229011	Longitudinal
229012	Transversal



Transversal osteotomy guide



Longitudinal osteotomy guide

K-FIX® – K-Wire End Protector

The K-Fix® pin protector is a simple system to protect patients or hospital staff from K-Wires sharp ends.

- Delivered sterile.

Reference	Length
119050	K-FIX® for K-WIRE – Dia. 0.8 mm to 2.0 mm (5 units per pack)



Weil Clamp

Reference	Length
119106	Weil Clamp

B-BOP® LOCK Plate

B-BOP®-LOCK plate is indicated for fixation of osteotomy of the basis of the first metatarsal. Examples include:

- Moderate to severe Hallux valgus.
- Hallux varus.


Implants

Reference	Description
320 100S	Basal plantar plate B-Bop® Lock right
320 200S	Basal plantar plate B-Bop® Lock left
295 110S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 10 mm
295 112S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 12 mm
295 114S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 14 mm
295 116S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 16 mm
295 118S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 18 mm
295 120S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 20 mm
295 122S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 22 mm
295 124S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 24 mm
295 126S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 26 mm
295 128S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 28 mm
295 130S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 30 mm
295 132S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 32 mm
295 134S	Screw and Lock screw titanium B-Bop® Lock Dia 3.0 x L 34 mm
195 100S	Lock screw B-Bop® Lock



Instrumentation

Reference	Description
219 027	Drilling guide Surfix Alpha Dia 2.0 mm
219 127	Screwdriver Torx T7
219 227	Screwdriver AO blade Torx T7
299 050	Drill AO Dia 2.0 mm
299 005	Drill Dia 2.0 mm
329 500	Bending forceps
329 002	Forceps
115 070	K-wire Dia 1.0 mm x L 70 mm
115 116	K-wire Dia 1.6 mm x L 150 mm
299 020	Depth gauge B-Bop Lock®
189 210	Wedge 10°
189 215	Wedge 15°
189 220	Wedge 20°

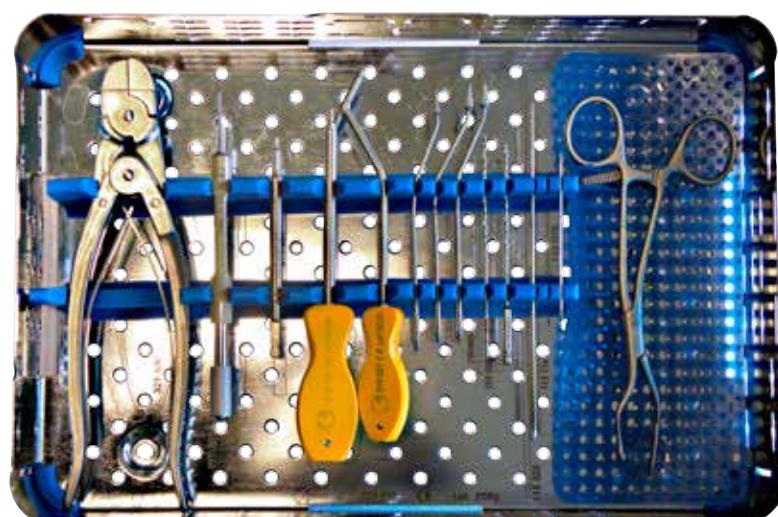

Container

Reference	Description
329 900	Container
including:	
329 901	Basis
329 902	Silicone mat
996200	Lid

IPP-ON® Interphalangeal Arthrodesis Implant

IPP-ON® interphalangeal implant is an implant which respects anatomical flexion to achieve interphalangeal arthrodesis of the lesser toes in case of:

- Fixed or semi-fixed hammer toe.
- Revision in case of arthrodesis or arthroplasty failure.
- Shortening in case of length excess of the second toe.
- Material: Stainless steel: 316 LVM.
- 2 sizes.



Reference	Description
230001S	IPP-ON® Interphalangeal Implant Size 1
230002S	IPP-ON® Interphalangeal Implant Size 2

IPP-ON® Instruments

Reference	Description
239011	Distal Hand Drill Size 1
239012	Proximal Hand Drill Size 1
239021	Distal Hand Drill Size 2
239022	Proximal Hand Drill Size 2
239500	Clamp
239030	Implant Holder

Sterilization Container

239000	IPP-ON® sterilization container including:
239001	Base
996100	Lid
278902	Mat
119909	Silicone wedge



METIS® Metatarso-Phalangeal Prosthesis

The three-component METIS® prosthesis replaces the articular surfaces of the great toe joint.

- Metatarsal component:
 - > 7 sizes (0 to 6).
 - > Material: Cobalt-Chromium alloy (CoCr).
 - > Coating: Porous Titanium & Hydroxyapatite (Ti and HAP).
- PE inlay:
 - > Ultra High Molecular Weight Polyethylene (UHMWPE).
 - > 5 sizes (1 to 5), 3 thicknesses (1 to 3).
- Phalangeal implant:
 - > 5 sizes (1 to 5).
 - > Material: Titanium alloy TA6V.
 - > Coating: Porous Titanium (Ti).



Reference	Description	Reference	Description
250100	Metatarsal component size 0	250204	Phalangeal component size 4
250101	Metatarsal component size 1	250205	Phalangeal component size 5
250102	Metatarsal component size 2	250311	METIS® Polyethylene Inlay - Size 1 - Thickness 1
250103	Metatarsal component size 3	250312	METIS® Polyethylene Inlay - Size 1 - Thickness 2
250104	Metatarsal component size 4	250313	METIS® Polyethylene Inlay - Size 1 - Thickness 3
250105	Metatarsal component size 5	250321	METIS® Polyethylene Inlay - Size 2 - Thickness 1
250106	Metatarsal component size 6	250322	METIS® Polyethylene Inlay - Size 2 - Thickness 2
250201	Phalangeal component size 1	250323	METIS® Polyethylene Inlay - Size 2 - Thickness 3
250202	Phalangeal component size 2	250331	METIS® Polyethylene Inlay - Size 3 - Thickness 1
250203	Phalangeal component size 3	250332	METIS® Polyethylene Inlay - Size 3 - Thickness 2
		250333	METIS® Polyethylene Inlay - Size 3 - Thickness 3
		250341	METIS® Polyethylene Inlay - Size 4 - Thickness 1
		250342	METIS® Polyethylene Inlay - Size 4 - Thickness 2
		250343	METIS® Polyethylene Inlay - Size 4 - Thickness 3
		250351	METIS® Polyethylene Inlay - Size 5 - Thickness 1
		250352	METIS® Polyethylene Inlay - Size 5 - Thickness 2
		250353	METIS® Polyethylene Inlay - Size 5 - Thickness 3


METIS® Instruments

METIS® Instruments

Reference	Description
139107	Metatarsal Osteotome
139120	Implant holder
139131	Locking screw
139210	Phalangeal reamer starter size
139211-215	Phalangeal reamer size 1 to 5
139140	Metatarsal sizer size 0
139121-126	Metatarsal sizer size 1 to 6
139150	Metatarsal cutting guide size 0
139111-116	Metatarsal cutting guide size 1 to 6
139216	Metatarsal impactor
139128	Visualization guide
139129	Visualization guide wire
119645	Screwdriver hexa 3.5 mm
119 601	Screwdriver hexa 2.5 mm
115216	K-Wire Dia. 1.6 x L. 150 mm
119611	Drill Dia. 2.5 x L. 150 mm
139940	METIS® sterilization container including:
139941	Metatarsal base
139942	Phalangeal base
139943	Base
139953	Lid
119909	Silicone wedge

METIS® Trial Implants

Reference	Description
139100-106	Metatarsal trial implant size 0 to 6
139311-313	Trial inlay size 1 thickness 1 to 3
139321-323	Trial inlay size 2 thickness 1 to 3
139331-333	Trial inlay size 3 thickness 1 to 3
139341-343	Trial inlay size 4 thickness 1 to 3
139351-353	Trial inlay size 5 thickness 1 to 3
139201-205	Phalangeal trial implant size 1 to 5

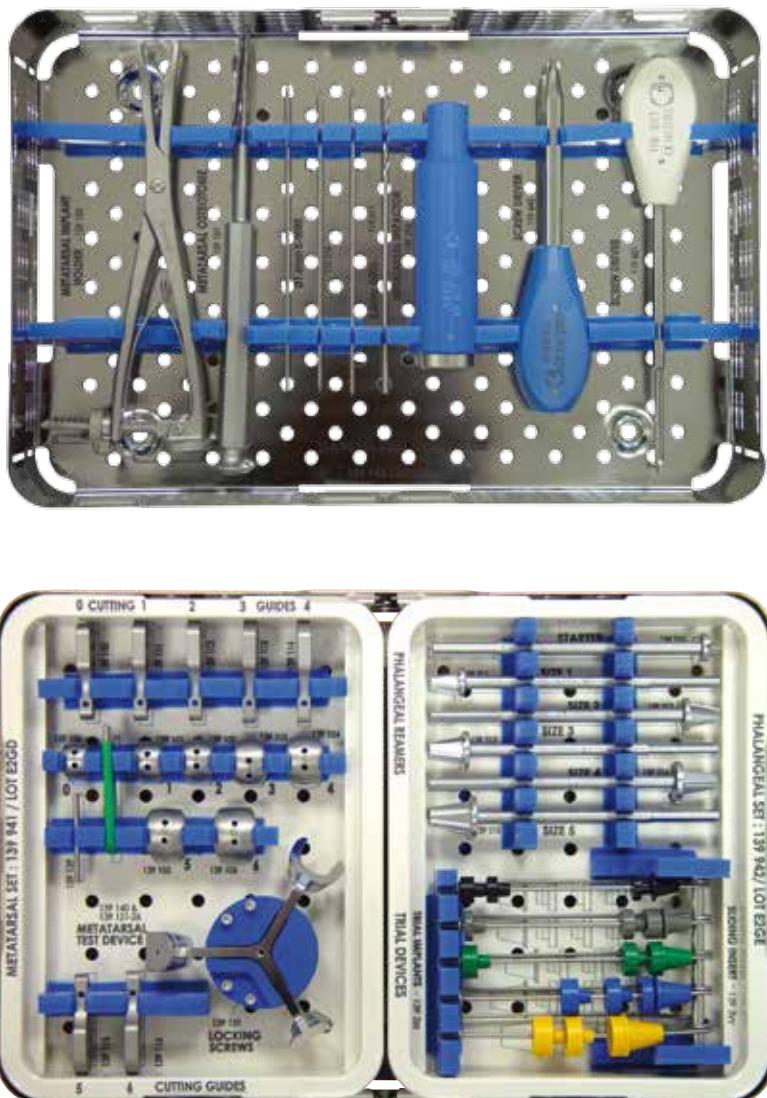

K2™ Hemi Toe Implant

The K2™ Hemi Toe Implant System is an anatomically designed, metallic, one-piece surface replacement system for the base of the hallux. 4 sizes are available.


K2™ Implants

Reference	Description
201010	Phalangeal, Size 1
201020	Phalangeal, Size 2
201030	Phalangeal, Size 3
201040	Phalangeal, Size 4



K2™ Instruments

Reference	Description
202010	Size 1 Trial
202020	Size 2 Trial
202030	Size 3 Trial
202040	Size 4 Trial
203010	Size 1 Shaper
203020	Size 2 Shaper
203030	Size 3 Shaper
203040	Size 4 Shaper
203100	Cutting Guide
203300	Sizer/Drill Guide
203500	Broach Handle
203600	Impactor
205000	Sterilization tray
203200	Reamer
203415	1.5 mm 80 mm drill bit

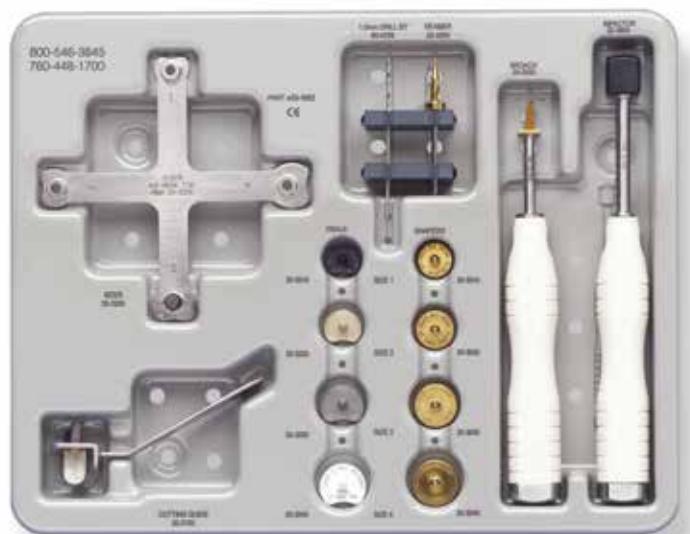

Movement Great Toe System

- Hemi Proximal Phalanx Implant.
- Hemi Metatarsal Implant.
- Total Great Toe Implant.

Reference	Description
MGT-890-10PPH	Hemi Proximal Phalanx, Size 10
MGT-890-20PPH	Hemi Proximal Phalanx, Size 20
MGT-890-30PPH	Hemi Proximal Phalanx, Size 30
MGT-890-40PPH	Hemi Proximal Phalanx, Size 40
MGT-890-10MT	Hemi Metatarsal, Size 10
MGT-890-20MT	Hemi Metatarsal, Size 20
MGT-890-30MT	Hemi Metatarsal, Size 30
MGT-890-40MT	Hemi Metatarsal, Size 40
MGT-890-10PPT	Phalangeal Total, Size 10
MGT-890-20PPT	Phalangeal Total, Size 20
MGT-890-30PPT	Phalangeal Total, Size 30
MGT-890-40PPT	Phalangeal Total, Size 40

Reference	Description
INS-890-00	Instrument Set
MIS-890-00	Metatarsal Implant Sizer
PIS-890-00	Proximal Phalanx Implant Sizer
GDW-890-00	Guide Pin, 2.0 mm X 125 mm
MSR-890-10/20	Metatarsal Surface Reamer, Size 10/20
MSR-890-30/40	Metatarsal Surface Reamer, Size 30/40
PSR-890-10/20	Proximal Phalanx Surface Reamer, Size 10/20
PSR-890-30/40	Proximal Phalanx Surface Reamer, Size 30/40
DRL-890-00	Cannulated Drill, 4.5 mm
DCC-890-00	Metatarsal Dorsal Cutting Guide
TRL-890-10MT	Metatarsal Trial, Size 10
TRL-890-20MT	Metatarsal Trial, Size 20
TRL-890-30MT	Metatarsal Trial, Size 30
TRL-890-40MT	Metatarsal Trial, Size 40
TRL-890-10PPH	Proximal Phalanx Hemi Trial, Size 10
TRL-890-20PPH	Proximal Phalanx Hemi Trial, Size 20
TRL-890-30PPH	Proximal Phalanx Hemi Trial, Size 30
TRL-890-40PPH	Proximal Phalanx Hemi Trial, Size 40
TRL-890-10PPT	Phalangeal Total Trial, Size 10
TRL-890-20PPT	Phalangeal Total Trial, Size 20
TRL-890-30PPT	Phalangeal Total Trial, Size 30
TRL-890-40PPT	Phalangeal Total Trial, Size 40
IMP-890-00MT	Metatarsal Impactor
IMP-890-00PP	Proximal Phalanx Impactor
ALG-890-00	Sizer Alignment Guide



HALLU®-FIX MTP Arthrodesis System


The HALLU®-FIX solution is a system dedicated to first MTP arthrodesis.

- Pre-bent plate.
- SNAP-OFF® screw fixation.
- Color coded.
- 3 sizes (3 left / 3 right).
- Material: Titanium alloy TA6V.

HALLU®-C Plate

HALLU®-C Plates

Reference	Description
117340(S)	HALLU®-C Plate Right-Size 1: L. 40 mm - 4 holes
117345(S)	HALLU®-C Plate Right-Size 2: L. 45 mm - 5 holes
117350(S)	HALLU®-C Plate Right-Size 3: L. 50 mm - 6 holes
117440(S)	HALLU®-C Plate Left-Size 1: L. 40 mm - 4 holes
117445(S)	HALLU®-C Plate Left-Size 2: L. 45 mm - 5 holes
117450(S)	HALLU®-C Plate Left-Size 3: L. 50 mm - 6 holes

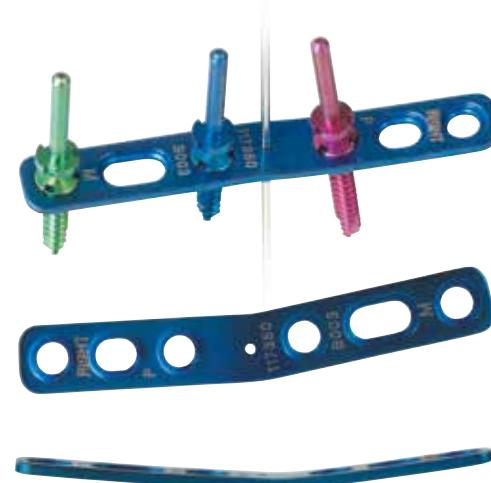

HALLU®-S Plate

HALLU®-S Plates

Reference	Description
117150(S)	HALLU®-S Plate Right-Size 1: L. 45 mm - 3 holes
117155(S)	HALLU®-S Plate Right-Size 2: L. 50 mm - 4 holes
117160(S)	HALLU®-S Plate Right-Size 3: L. 55 mm - 5 holes
117250(S)	HALLU®-S Plate Left-Size 1: L. 45 mm - 3 holes
117255(S)	HALLU®-S Plate Left-Size 2: L. 50 mm - 4 holes
117260(S)	HALLU®-S Plate Left-Size 3: L. 55 mm - 5 holes



HALLU[®] SNAP-OFF[®] Screws

- 2 diameters: 2.7 mm & 3.0 mm (for porous bone).
- Self-tapping.
- Color code for length identification.
- Material: Titanium alloy TA6V.

HALLU[®] Snap-Off[®] screws Dia. 3.0 mm

Reference	Length
117110(S)	10 mm
117112(S)	12 mm
117114(S)	14 mm
117116(S)	16 mm
117118(S)	18 mm

HALLU[®] Snap-Off[®] screws Dia. 2.7 mm

Reference	Length
117010(S)	10 mm
117012(S)	12 mm
117014(S)	14 mm
117016(S)	16 mm
117018(S)	18 mm
117020(S)	20 mm
117022(S)	22 mm
117024(S)	24 mm
117026(S)	26 mm
117028(S)	28 mm
117030(S)	30 mm
117032(S)	32 mm
117034(S)	34 mm



HALLU[®]-FIX Instruments



HALLU[®]-Rream Metatarsal



Reference	Diameter
129714	Dia. 14 mm
129716	Dia. 16 mm
129718	Dia. 18 mm
129720	Dia. 20 mm
129722	Dia. 22 mm

HALLU[®]-Rream Phalangeal

Reference	Diameter
129724	Dia. 14 mm
129726	Dia. 16 mm
129728	Dia. 18 mm
129730	Dia. 20 mm
129752	Dia. 22 mm

HALLU[®] Associated instruments

Reference	Description
129710	Quick coupling
129733	SNAP-OFF [®] Cannulated screwdriver - Dia. 2.7 mm and 3.0 mm
129731	Plate Bender Left
129732	Plate Bender Right
129734	Drilling Guide Dia. 1.9 mm
129735	Screwdriver tip
129736	Depth gauge
119618	Drill Dia. 1.9 x L. 100 mm
115216	K-Wire Dia. 1.6 x L. 150 mm
115100	K-Wire Dia. 1.0 x L. 100 mm

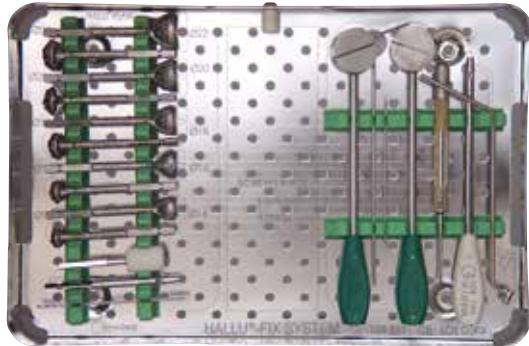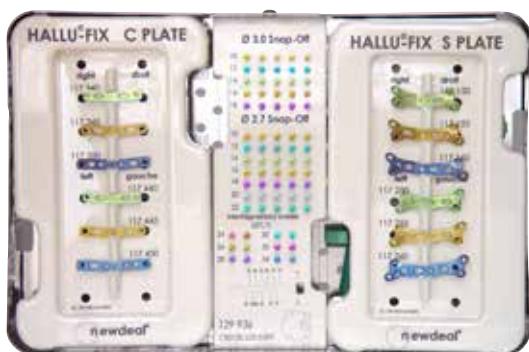

Sterilization container

129930	HALLU [®] -FIX Sterilization Container including:
129931	HALLU [®] -FIX Basis
129933	HALLU [®] -S Plate Insert
129932	HALLU [®] -C Plate Insert
996200	Lid
129936	HALLU [®] -FIX screws rack
119909	Silicone wedge (Optional)

(S) means available in sterile and non sterile

HALLU®-LOCK MTP Arthrodesis System

The HALLU®-LOCK solution is a locked system dedicated to first MTP arthrodesis:

Pre-bent plate.

- Color coded.
- 3 sizes (3 left / 3 right).
- Material: Titanium alloy TA 6V.
- Monobloc fixation with Surfix® locking system.

Surfix® locking screw

- 2 diameters: 2.7 mm & 3.0 mm (for porous bone).
- Standard and orientable screws.
- Color code for length identification.
- Material: Titanium alloy TA 6V.
- Sterily Packaged.



Surfix® standard screw
Dia. 2.7 mm + lock-screw

Reference	Length
285210S	10 mm
285212S	12 mm
285214S	14 mm
285216S	16 mm
285218S	18 mm
285220S	20 mm
285222S	22 mm
285224S	24 mm
285226S	26 mm
185200S	lock-screw

Surfix® Alpha
variable angle screw
Dia. 2.7 mm + lock-screw

Reference	Length
295210S	10 mm
295212S	12 mm
295214S	14 mm
295216S	16 mm
295218S	18 mm
295220S	20 mm
295222S	22 mm
295224S	24 mm
295226S	26 mm
195200S	lock-screw

Surfix® standard screw
Dia. 3.0 mm + lock-screw

Reference	Length
285110S	10 mm
285112S	12 mm
285114S	14 mm
285116S	16 mm
285118S	18 mm
285120S	20 mm
285122S	22 mm
285124S	24 mm
285126S	26 mm
185100S	lock-screw

Surfix® Alpha
variable angle screw
Dia. 3.0 mm + lock-screw

Reference	Length
295110S	10 mm
295112S	12 mm
295114S	14 mm
295116S	16 mm
295118S	18 mm
295120S	20 mm
295122S	22 mm
295124S	24 mm
295126S	26 mm
195100S	lock-screw

Hallu®-Lock C plate 10°

Reference	Description
290340S	Right-Size 1: L.40 mm – 4 holes
290345S	Right-Size 2: L.45 mm – 5 holes
290350S	Right-Size 3: L.50 mm – 6 holes
290440S	Left-Size 1: L.40 mm – 4 holes
290445S	Left-Size 2: L.45 mm – 5 holes
290450S	Left-Size 3: L.50 mm – 6 holes

Hallu®-Lock S plate 10°

Number of holes excludes the 4 extremity holes

Reference	Description
290150S	Right-Size 1: L.45 mm – 3 holes
290155S	Right-Size 2: L.50 mm – 3 holes
290160S	Right-Size 3: L.55 mm – 3 holes
290250S	Left-Size 1: L.45 mm – 3 holes
290255S	Left-Size 2: L.50 mm – 3 holes
290260S	Left-Size 3: L.55 mm – 3 holes

QWIX® transarticular compressive screw Dia. 3.0 mm

Reference	Length
111328S	28 mm
111330S	30 mm
111332S	32 mm
111334S	34 mm


HALLU[®]-LOCK Instruments

HALLU[®]-REAM System

129714	Metatarsal Reamer Dia. 14 mm
129716	Metatarsal Reamer Dia. 16 mm
129718	Metatarsal Reamer Dia. 18 mm
129720	Metatarsal Reamer Dia. 20 mm
129722	Metatarsal Reamer Dia. 22 mm
129724	Phalangeal Reamer Dia. 14 mm
129726	Phalangeal Reamer Dia. 16 mm
129728	Phalangeal Reamer Dia. 18 mm
129730	Phalangeal Reamer Dia. 20 mm
129752	Phalangeal Reamer Dia. 22 mm

HALLU[®]-Lock associated instruments

129710	Quick coupling
997100	Quick-Coupling AO
299070	Left bender
299080	Right bender
219027	SURFIX [®] Alpha drilling guide Dia. 2.0 mm
219627	SURFIX [®] drilling guide Dia. 2.0 mm
219127	Screwdriver torx T7
219227	AO Screwdriver tip torx T7
299020	Depth Gauge
119133	Handle with AO Attachment Dia. 3.0 mm
119135	AO Screwdriver tip dia 3.0 mm
299010	Trial plate holder
299150	Trial plate-S Right - Size 1
299155	Trial plate-S Right - Size 2
299160	Trial plate-S Right - Size 3
299250	Trial plate-S Left - Size 1
299255	Trial plate-S Left - Size 2
299260	Trial plate-S Left - Size 3
299340	Trial plate-C Right - Size 1
299345	Trial plate-C Right - Size 2
299350	Trial plate-C Right - Size 3
299440	Trial plate-C Left - Size 1
299445	Trial plate-C Left - Size 2
299450	Trial plate-C Left - Size 3
299005	Drill Dia. 2.0 x L. 100 mm
299050	AO Drill AO Dia. 2.0 x L. 100 mm
159027S	2 in 1 cannulated drill AO dia 2.2/3.0 x L. 12 mm sterile
115070	K-Wire Dia. 1.0 x L. 70 mm
115100	K-wire Dia. 1.0 x L. 100 mm
115116	K-Wire Dia. 1.6 x L. 150 mm

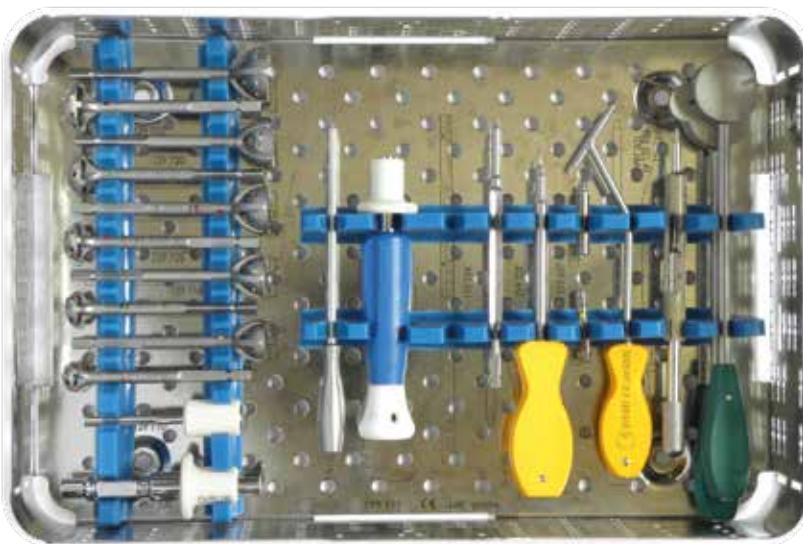

HALLU[®]-LOCK sterilization container

299900	HALLU [®] -Lock sterilization container
299901	Base
299903	Trial implants tray
299904	K-Wire tray
996200	Lid
119909	Silicone wedge

HALLU[®]-REAM Set

Reference	Description
129714	Metatarsal Reamer Dia. 14 mm
129716	Metatarsal Reamer Dia. 16 mm
129718	Metatarsal Reamer Dia. 18 mm
129720	Metatarsal Reamer Dia. 20 mm
129722	Metatarsal Reamer Dia. 22 mm
129724	Phalangeal Reamer Dia. 14 mm
129726	Phalangeal Reamer Dia. 16 mm
129728	Phalangeal Reamer Dia. 18 mm
129730	Phalangeal Reamer Dia. 20 mm
129752	Phalangeal Reamer Dia. 22 mm

Instruments	
129710	Quick coupling
115216	K-Wire Dia. 1.6 x L. 150 mm

Sterilization container	
129935	HALLU [®] -Ream sterilization container including:
129938	HALLU [®] -Ream Basis
996100	Lid



DPR System Minimal Invasive Foot Surgery

DPR System minimal invasive foot surgery was born from our collaboration with minimal invasive foot surgeons.

- Single use: Sterile packaging.
- Safety: Protection by silicone ring.
- Identification: Color coded.
- Material: Stainless Steel 316L.



DPR System Minimal Invasive Foot Surgery burrs

278002S	Burr straight Dia. 2.0 x L. 15 mm
278007S	Burr conical Dia. 3.1/1.0 x L. 12 mm
278005S	Burr straight Dia. 1.9 x L. 10 mm
278008S	Burr conical Dia. 4.1/1.0 x L. 12 mm
278009S	Burr cylindrical Dia. 4.1 x L. 15 mm
278010S	Burr cylindrical Dia. 3.1 x L. 15 mm

DPR System Minimal Invasive Foot Surgery curettes

278121	Curette Medium - Down
278122	Curette Medium - Up
278123	Curette Large - Down
278124	Curette Large - Up
278100	Sleeve protection Cap
278110	Sleeve protection Dia. 3.1 mm
278109	Sleeve protection Dia. 4.1 mm

Sterilization container

278900	DPR System Minimal Invasive Foot Surgery sterilization container
278901	Base
996100	Lid
278902	Mat
119909	Silicone wedge



Please contact us if you need a MIS motor offer.

Post-Operative Shoes


Reference	Description
Flat Post Operative Shoe	
999001	Small
999002	Medium
999003	Large
999004	X-Large



Reference	Description
Wedged Hell Post Operative Shoe	
999100	Size 4 to 6.5
999101	Size 7 to 8.5
999102	Size 9 to 10.5



250
240
230
220
210
200
190
180
170
160
150
140
130
120
110
100
90
80
70
60
50
40
30
20
10
0
MILLIMETERS

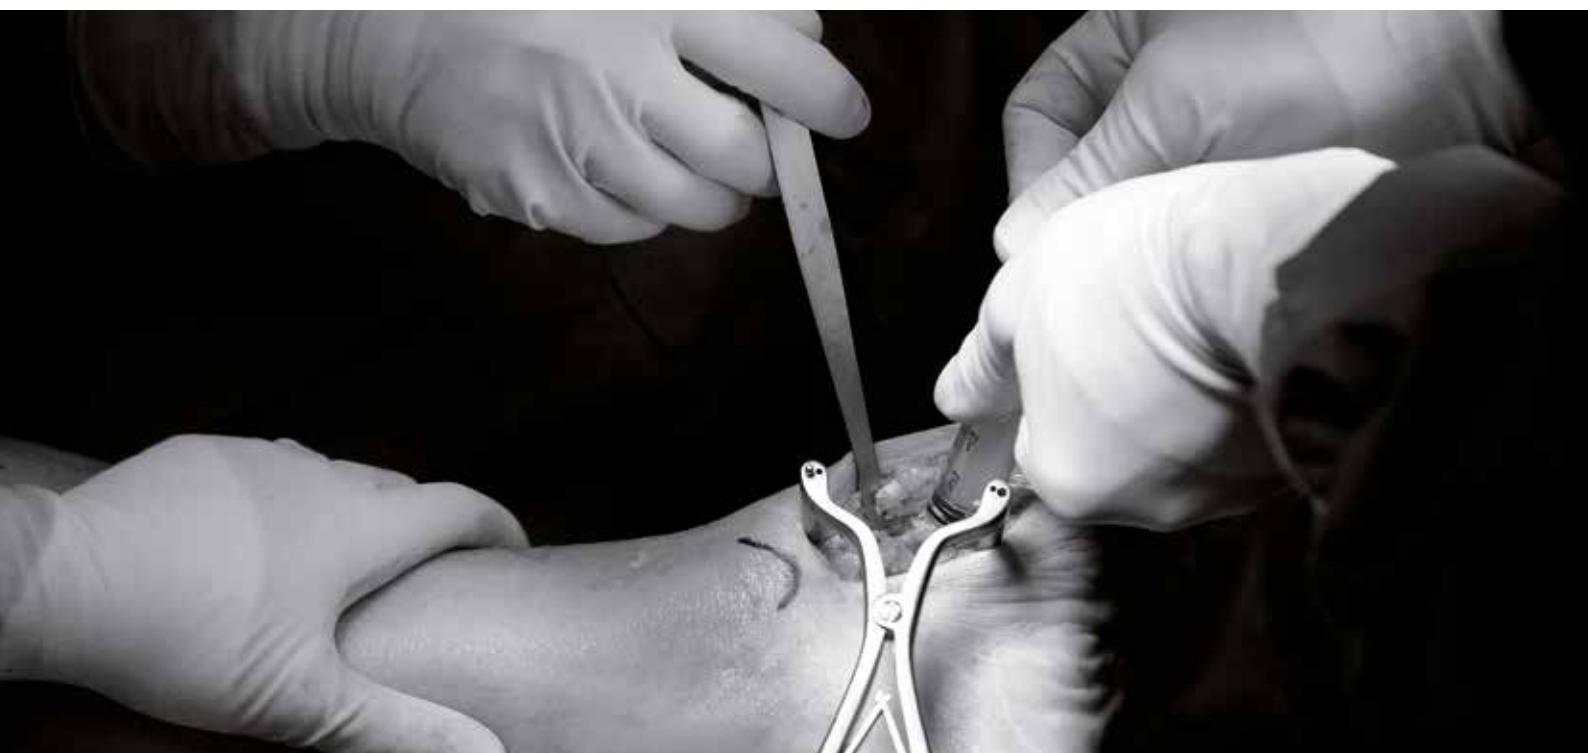

Integra® Mid & HindFoot Solutions

QWIX® Fixation Screw, dia. 4.3 mm

For the fixation of bone fractures or for bone reconstruction.

- Self-drilling and self-tapping.
- Intra-osseous fixation.
- Variable lag length for extremity fixation.
- Material: Titanium alloy TA6V.

QWIX® dia. 4.3 mm

Reference	Length
111422S	L. 22 mm
111424S	L. 24 mm
111426S	L. 26 mm
111428S	L. 28 mm
111430S	L. 30 mm
111432S	L. 32 mm
111434S	L. 34 mm
111436S	L. 36 mm
111438S	L. 38 mm
111440S	L. 40 mm
111445S	L. 45 mm
111450S	L. 50 mm
111455S	L. 55 mm
111460S	L. 60 mm




QWIX® dia. 4.3 mm Instruments

Reference	Description
119104	Screwdriver tip
119139	Short Drill dia. 2.6/5.0 x L. 100 mm
119138	Quick coupling handle
119516	Long cannulated drill dia. 2.6 x L. 140 mm
115116	K-Wire dia. 1.6 x L. 150 mm

Sterilization container

Reference	Description
119935	QWIX® 4.3 sterilization container including:
119937	Cylinder
119936	Base
119938	Mat
996400	Lid

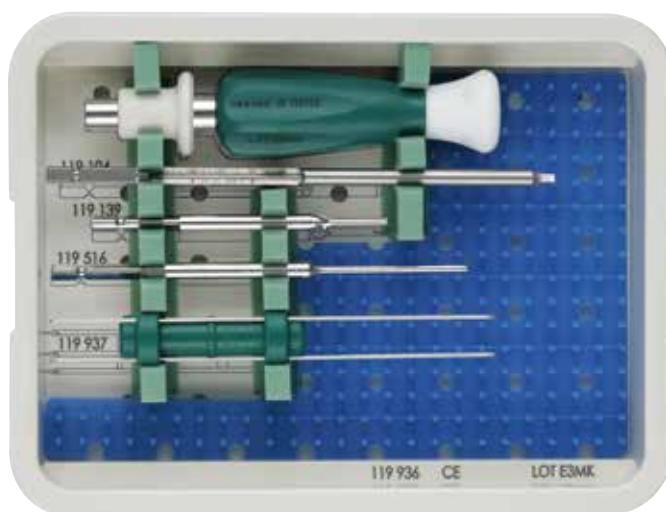

Large QWIX® Fixation and Positioning Screws dia. 5.5 mm / 7.5 mm

- Fixation and positioning screws dia. 5.5 and 7.5 mm.
- Self-drilling and self-tapping.
- Intra-osseous fixation.
- Material: Titanium alloy TA6V.
- Sterile packaged.

Large QWIX® Fixation screws
dia. 7.5 mm



Large QWIX® Positioning screws
dia. 7.5 mm



Reference	Length
111740S	L. 40 mm
111745S	L. 45 mm
111750S	L. 50 mm
111755S	L. 55 mm
111760S	L. 60 mm
111765S	L. 65 mm
111770S	L. 70 mm
111775S	L. 75 mm
111780S	L. 80 mm
111785S	L. 85 mm
111790S	L. 90 mm
111795S	L. 95 mm
111800S	L. 100 mm
111805S	L. 105 mm
111810S	L. 110 mm
111815S	L. 115 mm
111820S	L. 120 mm


Reference	Length
111530S	L. 30 mm
111535S	L. 35 mm
111540S	L. 40 mm
111545S	L. 45 mm
111550S	L. 50 mm
111555S	L. 55 mm
111560S	L. 60 mm
111565S	L. 65 mm
111570S	L. 70 mm
111575S	L. 75 mm
111580S	L. 80 mm

Reference	Length
121740S	L. 40 mm
121745S	L. 45 mm
121750S	L. 50 mm
121755S	L. 55 mm
121760S	L. 60 mm
121765S	L. 65 mm
121770S	L. 70 mm
121775S	L. 75 mm
121780S	L. 80 mm
121785S	L. 85 mm
121790S	L. 90 mm
121795S	L. 95 mm
121800S	L. 100 mm
121805S	L. 105 mm
121810S	L. 110 mm
121815S	L. 115 mm
121820S	L. 120 mm

Reference	Length
121530S	L. 30 mm
121535S	L. 35 mm
121540S	L. 40 mm
121545S	L. 45 mm
121550S	L. 50 mm
121555S	L. 55 mm
121560S	L. 60 mm
121565S	L. 65 mm
121570S	L. 70 mm
121575S	L. 75 mm
121580S	L. 80 mm

Large QWIX® Instruments

Reference	Length
119150	Measurer 200 and 250 mm
119151	Internal protection sleeve dia. 1.8 mm
119152	Drilling guide dia. 4.5 mm
119153	External protection sleeve dia. 7.3 mm
119154	Cannulated drill dia. 1.8/4.2 x L. 180 mm
119155	Cannulated 2 in 1 drill dia. 4.2/5.8 x L. 113 mm
119156	Hexa screwdriver Tip 3 mm
119171	Internal protection sleeve dia. 2.7 mm
119172	Drilling guide dia. 5.8 mm
119173	External protection sleeve dia. 9.3 mm
119174	Cannulated drill dia. 2.7/5.5 x L. 210 mm
119175	Cannulated 2 in 1 drill dia. 5.5/7.0 x L. 128 mm
119176	Hexa screwdriver Tip 4 mm
119177	T handle quick coupling
115516	K-Wire dia. 1.6 x L. 200 mm
529061	K-Wire dia. 2.5 x L. 250 mm

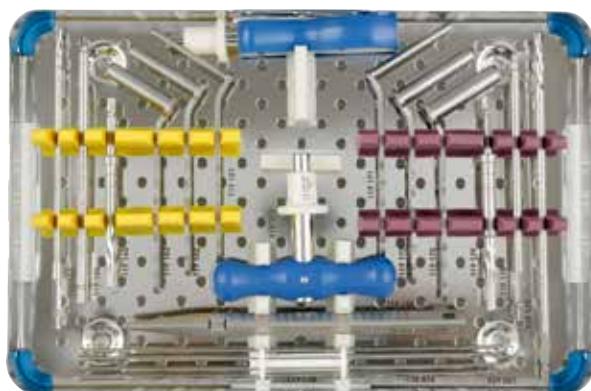

Sterilization container

Reference	Description
121950	LARGE QWIX® sterilization container including:
121951	Base
996200	Lid
119170	Cylinder
119909	Silicone wedge

I.CO.S.® Ideal Compression Screw

Cannulated Titanium 4.0 mm and 6.5 mm diameter compression screw are dedicated to fixation of osteotomies or for fractures stabilization.

- K-Wire guidance for drilling, tapping and screw setting (dia. 1.6 or 2.5 mm).
- Adjustable and controlled static compression.
- Dynamic compression by additional head screwing.
- Intra osseous implant.
- Large range of sizes :
 - > I.CO.S.® dia. 4.0 mm:
 - » L. 26 to 40 mm by 2 mm
 - » L. 40 to 60 mm by 5 mm
 - > I.CO.S.® dia. 6.5 mm:
 - » L. 40 to 90 mm by 5 mm
- Material: Titanium alloy TA6V.
- Cortico-spongious thread.
- Long non threaded shaft (lag screws) allowing compression.



I.CO.S.® dia. 4.0 mm

Reference	Length
105426	L. 26 mm
105428	L. 28 mm
105430	L. 30 mm
105432	L. 32 mm
105434	L. 34 mm
105436	L. 36 mm
105438	L. 38 mm
105440	L. 40 mm
105445	L. 45 mm
105450	L. 50 mm
105455	L. 55 mm
105460	L. 60 mm




I.CO.S.® dia. 6.5 mm

Reference	Length
105640	L. 40 mm
105645	L. 45 mm
105650	L. 50 mm
105655	L. 55 mm
105660	L. 60 mm
105665	L. 65 mm
105670	L. 70 mm
105675	L. 75 mm
105680	L. 80 mm
105685	L. 85 mm
105690	L. 90 mm

I.C.O.S.® dia. 4.0 mm Instruments

Reference	Description
119501	Protection Sleeve dia. 6 mm
119506	Drilling Guide dia. 1.8 mm
119510	Measurer
119516	Long cannulated drill dia. 2.6 x L. 140 mm
119522	Short cannulated Drill dia. 5.0 x L. 110 mm
129710	Quick-coupling
119525	Tap
119531	Internal screwdriver dia. 4.0 x L. 100 mm
119532	Screwdriver tip dia. 4.0 x L. 100 mm
119536	External screwdriver dia. 6.4 x L. 170 mm

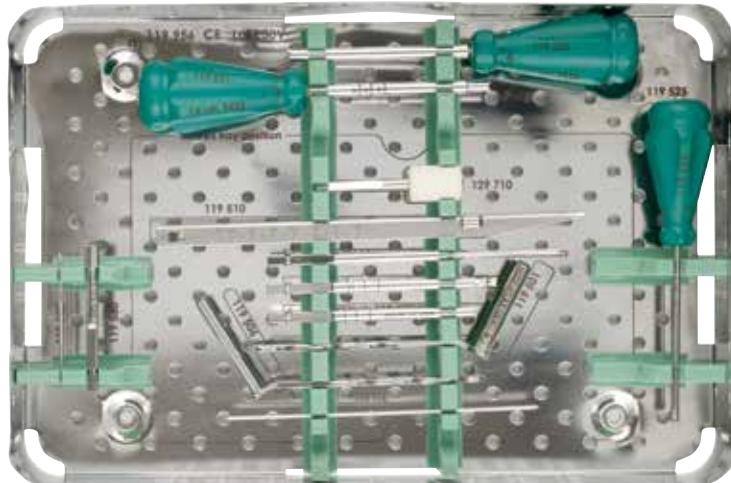


I.C.O.S.® 4.0 sterilization Container

Reference	Description
119974	I.C.O.S.® 4.0 sterilization container including:
119956	Base
119951	Screw rack
119949	Metallic lid for screws (Optional)
996200	Lid
119909	Silicone wedge

I.C.O.S.® dia. 6.5 mm Instruments

Reference	Description
119541	Drilling Guide dia. 6.5 x L. 100 mm
119551	Internal protection sleeve dia. 6.5 mm
119552	External protection sleeve dia. 6.5 mm
119576	Long cannulated drill dia. 4.6 x L. 180 mm
119546	Short cannulated drill dia. 6.5 x L. 118 mm
119561	Internal screwdriver dia. 6.5 x L. 170 mm
119562	Screwdriver tip dia. 6.5 x L. 110 mm
119566	External screwdriver dia. 10.1 x L. 170 mm
119555	Tap
119510	Measurer
129710	Quick coupling
115225	K-Wire dia. 2.5 x L. 200 mm

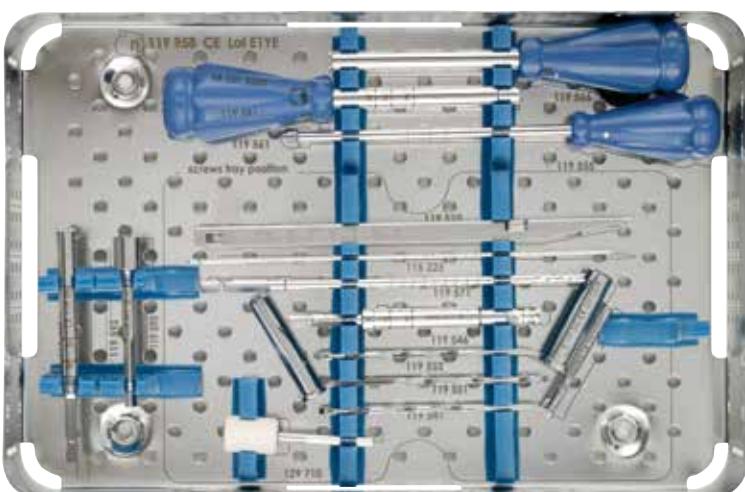

I.CO.S.® 6.5 sterilization Container

Reference	Description
119976	I.C.O.S.® 6.5 sterilization Container including:
119958	Base
119953	Screws rack
119949	Metallic lid for screws (Optional)
119957	Lid
119909	Silicone wedge

I.CO.S.® Removal Set

This removal set contains instrumentation required to remove I.CO.S.® screws dia. 4.0 and 6.5 mm

Removal set Instruments (for all diameters)

Reference	Description
Instruments for I.CO.S.® dia. 4.0 mm	
115116	K-Wire dia. 1.6 x L. 150 mm
119531	Internal screwdriver dia. 4.0 x L. 100 mm
119580	Trephine dia. 4.0 x L. 70 mm
119582	Internal Extractor dia. 4.0 x L. 60 mm (single use)
Instruments for I.CO.S.® dia. 6.5 mm	
115225	K-Wire dia. 2.5 x L. 200 mm
119561	Internal screwdriver dia. 6.5 x L. 170 mm
119590	Trephine dia. 6.5 x L. 80 mm
119592	Internal Extractor dia. 6.5 x L. 70 mm (single use)



Sterilization container

Reference	Description
119975	I.CO.S.® Removal Sterilization container including
119959	Lid
119955	Base
119977	K-Wire cylinder

KALIX® II Flat Foot Implant

Expansion endorthesis for flat foot correction in child or adult.

Progressive expansion.

- Material:
 - > Titanium alloy TA6V
 - > Polyethylene (UHMWPE)
- Color coded.
- Sterily packaged.

Reference	Ext. diameter
141009	dia. 9 mm
141010	dia. 10 mm
141011	dia. 11 mm
141012	dia. 12 mm
141013	dia. 13 mm
141014	dia. 14 mm
141015	dia. 15 mm
141017	dia. 17 mm



KALIX® II Flat Foot Implant Instruments

Reference	Description
119825	Viladot Lever
119850	Impactor
119831	Trial implant holder
119859	KALIX® II Trial implant dia. 9.0 mm
119860	KALIX® II Trial implant dia. 10.0 mm
119861	KALIX® II Trial implant dia. 11 mm
119862	KALIX® II Trial implant dia. 12 mm
119863	KALIX® II Trial implant dia. 13 mm
119864	KALIX® II Trial implant dia. 14 mm
119865	KALIX® II Trial implant dia. 15 mm
119867	KALIX® II Trial implant dia. 17 mm



KALIX® II sterilization container

Reference	Description
119880	KALIX® II sterilization container including
119882	Lid
119881	Base

MBA™ Titanium Subtalar Implant

The Subtalar MBA™ System is indicated for use in treatment of the hyperpronated foot and stabilization of the subtalar joint. It is designed to block the posterior and inferior displacement of the talus, thus allowing normal subtalar joint motion while blocking excessive pronation and the resulting sequela.

- Severely pronated foot.
- Walking intemperance.
- Calcaneal stance position greater than 5°.
- Manually correctable deformities.
- Mid-tarsal breech (arch pain).
- Forefoot varus greater than 10°.



Removal set Instruments (for all diameters)

Reference	Description
Instruments tray	
05-0016	Guide pin insert holder
05-0206	Trial 6 mm
05-0208	Trial 8 mm
05-0209	Trial 9 mm
05-0210	Trial 10 mm
05-0212	Trial 12 mm
05-1002	Yellow probe
05-1006	6 mm Sizer
05-1008	8 mm Sizer
05-1009	9 mm Sizer
05-1010	10 mm Sizer
05-1012	12 mm Sizer
05-1020	Insertion Device
05-0017	Guide pin 2 mm
05-5001	Sterilization tray
Implants	
05-0106	MBA™ 6 mm implant
05-0108	MBA™ 8 mm implant
05-0109	MBA™ 9 mm implant
05-0110	MBA™ 10 mm implant
05-0112	MBA™ 12 mm implant



ADVANSYS® Dorsal Lisfranc Plate

The Dorsal Lisfranc Plates are intended for fractures, fusions, osteotomies and replantations of small bones at the tarso-metatarsal joints (Lisfranc joints).

- 3 sizes of implants:
3 right & 3 left plates
(small, medium and large).
- 3.5 mm diameter screws available in lengths from 8 mm to 34 mm in 2 mm increments.
- 3.5 mm lock-screws.
- Material:
➤ Plate: Stainless Steel 316LVM.
➤ Screw: Titanium TA6V.



ADVANSYS® Dorsal Lisfranc Plates

Reference	Description
181021S	ADVANSYS® DLP small-right
181022S	ADVANSYS® DLP medium-right
181023S	ADVANSYS® DLP large-right
181031S	ADVANSYS® DLP small-left
181032S	ADVANSYS® DLP medium-left
181033S	ADVANSYS® DLP large-left

Surfix® Locking screw Sterile Titanium dia.3.5 mm + lock-screw

Reference	Description
285310S	L. 10 mm
285312S	L. 12 mm
285314S	L. 14 mm
285316S	L. 16 mm
285318S	L. 18 mm
285320S	L. 20 mm
285322S	L. 22 mm
285324S	L. 24 mm
285326S	L. 26 mm
285328S	L. 28 mm
285330S	L. 30 mm
285332S	L. 32 mm
285334S	L. 34 mm
185300S	Lock-screw dia.3.5 mm

Optional instrument

Reference	Description
MA3511	Surfix® screw extractor 3.5 mm

ADVANSYS® Medial Lisfranc Plate

The Medial Lisfranc Plates are intended to be used for bone fixation such as:

- Lisfranc arthrodesis.
- Mono or bi-cortical osteotomies or fractures near the 1st metatarso-cuneiform joint.
- 2 sizes of implants:
2 right & 2 left plates (small and large sizes).
- 3.5 mm diameter screws available in lengths from 8 mm to 34 mm in 2 mm increments.
- 3.5 mm lock-screws.
- Material:
➤ Plate: Stainless Steel 316LVM.
➤ Screw: Titanium TA6V.
- Sterily packaged.



ADVANSYS® Medial Lisfranc Plate

Reference	Description
181041S	ADVANSYS® MLP small-right
181042S	ADVANSYS® MLP large-right
181051S	ADVANSYS® MLP small-left
181052S	ADVANSYS® MLP large-left

Surfix® Locking screw Sterile Titanium dia. 3.5 mm + lock-screw

Reference	Description
285310S	L. 10 mm
285312S	L. 12 mm
285314S	L. 14 mm
285316S	L. 16 mm
285318S	L. 18 mm
285320S	L. 20 mm
285322S	L. 22 mm
285324S	L. 24 mm
285326S	L. 26 mm
285328S	L. 28 mm
285330S	L. 30 mm
285332S	L. 32 mm
285334S	L. 34 mm
185300S	Lock-screw dia.3.5 mm

Optional instrument

Reference	Description
MA3511	Surfix® screw extractor 3.5 mm

ADVANSYS® Medial Lisfranc Plate Instruments

Reference	Description
115100	K-Wire dia. 1.0 x L. 100 mm
219335	Depth gauge hole dia. 3.5 mm
219435	AO Screwdriver tip hexa 2.0 x L. 76 mm
219535	AO drill dia. 2.7 x L. 125 mm
219635	Drilling guide dia. 2.7 mm
219735	Bending forceps L. 171 hole - dia 3.5 mm
219835	Screwdriver hexa 2.0 x L. 180 mm
169041	MLP trial implant right-small
169042	MLP trial implant right-large
169051	MLP trial implant left-small
169052	MLP trial implant left-large

ADVANSYS® Midfoot sterilization container


Reference	Description
169102	ADVANSYS® Midfoot sterilization container includes:
169112	Base
996200	Lid
169106	Cylinder
169107	DLP/MLP Trial implant module
119909	Silicone wedge

DLP trial plates

Reference	Description
169021	Dorsal trial plate, right, small
169022	Dorsal trial plate, right, medium
169023	Dorsal trial plate, right, large
169031	Dorsal trial plate, left, small
169032	Dorsal trial plate, left, medium
169033	Dorsal trial plate, left, large

Optional instrument

Reference	Description
MA3511	Surfix® screw extractor 3.5 mm

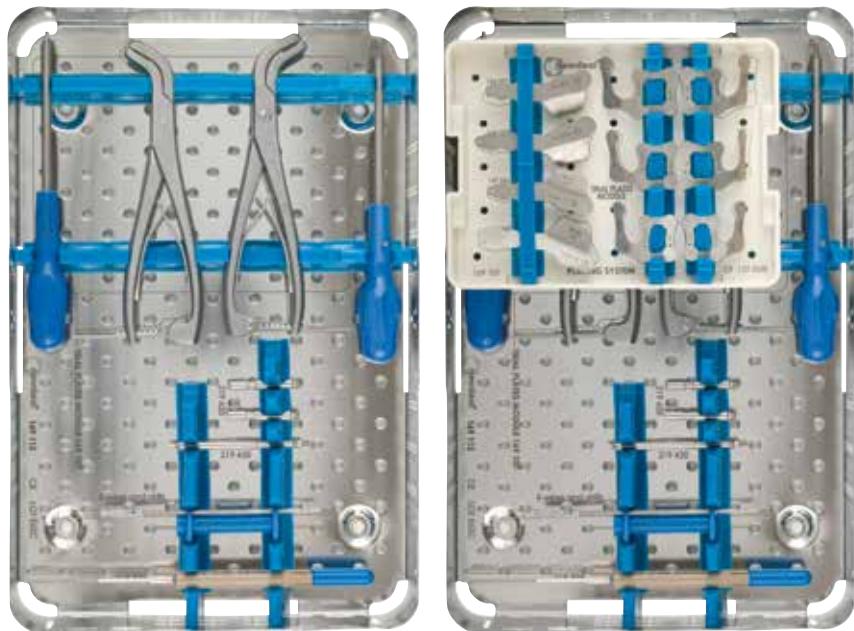

UNI-CP™ Compression plate

The UNI-CP™ compression plate is indicated for fixation of bone fractures or for bone reconstruction:

- 4 plate configurations:
 - > 2 hole design (17, 20, 25, and 30 mm interaxis)
 - > 4 hole design (20, 25, and 30 mm interaxis)
 - > 4 hole T-shape design (20 mm interaxis)
 - > 4 hole U-shape design (17x20, 19x22.5, 21x25 mm interaxis)
- Range of screw lengths: from 12 mm to 40 mm in 2 mm increments.
- Surfix® Locking Technology.
- Material
 - > Plate: Stainless Steel 316LVM.
 - > Screw: Titanium TA6V.



UNI-CP™ plate 4 holes



UNI-CP™ plate 2 holes



CP T-shape plate



UNI-CP™ U-shape plate

Surfix® Sterile Titanium screw
dia. 3.5 mm + lock-screw

UNI-CP™ Compression Plate

Reference	Description
330430S	UNI-CP™ 4 holes - 30 mm
330425S	UNI-CP™ 4 holes - 25 mm
330420S	UNI-CP™ 4 holes - 20 mm
330230S	UNI-CP™ 2 holes - 30 mm
330225S	UNI-CP™ 2 holes - 25 mm
330220S	UNI-CP™ 2 holes - 20 mm
330217S	UNI-CP™ 2 holes - 17 mm
330030S	UNI-CP™ T shaped plate
330021S	4 holes - 17x20 mm U shaped plate
330023S	4 holes - 19x22.5 mm U shaped plate
330025S	4 holes - 21x25 mm U shaped plate


Reference	Description
285312S	L. 12 mm
285314S	L. 14 mm
285316S	L. 16 mm
285318S	L. 18 mm
285320S	L. 20 mm
285322S	L. 22 mm
285324S	L. 24 mm
285326S	L. 26 mm
285328S	L. 28 mm
285330S	L. 30 mm
285332S	L. 32 mm
285334S	L. 34 mm
285336S	L. 36 mm
285338S	L. 38 mm
285340S	L. 40 mm
185300S	Surfix® lock screw dia. 3.5 mm

Optional instrument

Reference	Description
MA3511	Surfix® screw extractor 3.5 mm

UNI-CP™ Compression plate Instruments

Reference	Description
219335	Depth gauge hole dia. 3.5 mm
219435	AO Screwdriver tip hexa 2.0 x L. 76 mm
219535	AO drill dia. 2.7 x L. 125 mm
219635	Drilling guide dia. 2.7 mm
219735	Bending forceps L. 171 hole - dia 3.5 mm
219835	Screwdriver hexa 2.0 x L. 180 mm
339001	Compression forceps
339004	Trial implant for T and U plates
339005	Trial implant for 2 and 4 holes plates
339003	Holder
115101	K-Wire dia. 1.0 x L. 100 mm

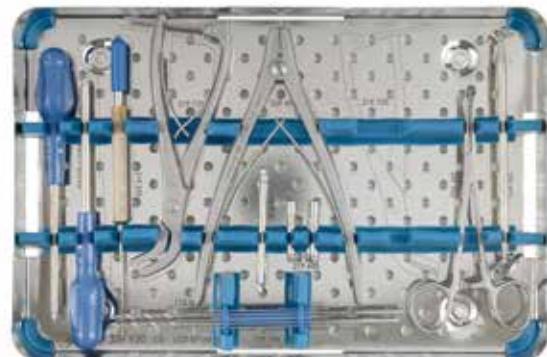

UNI-CP™ sterilization container

Reference	Description
339950	UNI-CP™ sterilization container including:
996200	Lid
339920	Base
169106	Cylinder
119909	Silicone wedge

Optional instrument

Reference	Description
MA3511	Surfix® screw extractor 3.5 mm

HINTEGRA® Total Ankle Prosthesis – Primary Surgery

The HINTEGRA® Total Ankle Prosthesis is a three components design anatomical prosthesis.

- Materials:
 - > Talar & tibial components:
Cobalt Chromium alloy (CoCr), with double coating:
 - » Porous Titanium & Hydroxyapatite (Ti and HAP),
for optimal bone ingrowth (osteointegration).
 - > PE inlay: UHMWPE.
 - > Fixation screws (optional): Stainless steel M30NW.



HINTEGRA® Total Ankle Prosthesis – Tibial Component – Primary Surgery

Minimum contact stress to the bone.

- Materials:
 - > Cobalt Chromium alloy (CoCr) with double coating:
Porous Titanium & Hydroxyapatite (Ti and HAP),
for optimal bone ingrowth (osteointegration).
- 7 sizes right & 7 sizes left.

Reference Description

HINTEGRA® - Tibial Component - Right

301200	HINTEGRA® tibial component-right - size 0
301201	HINTEGRA® tibial component-right - size 1
301202	HINTEGRA® tibial component-right - size 2
301203	HINTEGRA® tibial component-right - size 3
301204	HINTEGRA® tibial component-right - size 4
301205	HINTEGRA® tibial component-right - size 5
301206	HINTEGRA® tibial component-right - size 6



HINTEGRA® - Tibial Component - Left

302200	HINTEGRA® tibial component-left - size 0
302201	HINTEGRA® tibial component-left - size 1
302202	HINTEGRA® tibial component-left - size 2
302203	HINTEGRA® tibial component-left - size 3
302204	HINTEGRA® tibial component-left - size 4
302205	HINTEGRA® tibial component-left - size 5
302206	HINTEGRA® tibial component-left - size 6

HINTEGRA® Total Ankle Prosthesis – PE Inlay – Primary Surgery

- Ultra High Molecular Weight Polyethylene (UHMWPE).
- X-rays markers (Titanium TA6V rods).
- Same size as talar component: 6 sizes with 4 thicknesses (5, 6, 7, 9 mm).

HINTEGRA® - PE inlay - size 0	
300005	HINTEGRA® PE inlay - size 0 - thickness 5 mm
300006	HINTEGRA® PE inlay - size 0 - thickness 6 mm
300007	HINTEGRA® PE inlay - size 0 - thickness 7 mm
300009	HINTEGRA® PE inlay - size 0 - thickness 9 mm
HINTEGRA® - PE inlay - size 1	
300105	HINTEGRA® PE inlay - size 1 - thickness 5 mm
300106	HINTEGRA® PE inlay - size 1 - thickness 6 mm
300107	HINTEGRA® PE inlay - size 1 - thickness 7 mm
300109	HINTEGRA® PE inlay - size 1 - thickness 9 mm
HINTEGRA® - PE inlay - size 2	
300205	HINTEGRA® PE inlay - size 2 - thickness 5 mm
300206	HINTEGRA® PE inlay - size 2 - thickness 6 mm
300207	HINTEGRA® PE inlay - size 2 - thickness 7 mm
300209	HINTEGRA® PE inlay - size 2 - thickness 9 mm
HINTEGRA® - PE inlay - size 3	
300305	HINTEGRA® PE inlay - size 3 - thickness 5 mm
300306	HINTEGRA® PE inlay - size 3 - thickness 6 mm
300307	HINTEGRA® PE inlay - size 3 - thickness 7 mm
300309	HINTEGRA® PE inlay - size 3 - thickness 9 mm

HINTEGRA® - PE inlay - size 4	
300405	HINTEGRA® PE inlay - size 4 - thickness 5 mm
300406	HINTEGRA® PE inlay - size 4 - thickness 6 mm
300407	HINTEGRA® PE inlay - size 4 - thickness 7 mm
300409	HINTEGRA® PE inlay - size 4 - thickness 9 mm
HINTEGRA® - PE inlay - size 5	
300505	HINTEGRA® PE inlay - size 5 - thickness 5 mm
300506	HINTEGRA® PE inlay - size 5 - thickness 6 mm
300507	HINTEGRA® PE inlay - size 5 - thickness 7 mm
300509	HINTEGRA® PE inlay - size 5 - thickness 9 mm
HINTEGRA® - PE inlay - size 6	
300605	HINTEGRA® PE inlay - size 6 - thickness 5 mm
300606	HINTEGRA® PE inlay - size 6 - thickness 6 mm
300607	HINTEGRA® PE inlay - size 6 - thickness 7 mm
300609	HINTEGRA® PE inlay - size 6 - thickness 9 mm



HINTEGRA® Total Ankle Prosthesis – Talar component with Pegs – Primary Surgery

- Double coating: Porous Titanium & Hydroxyapatite (Ti and HAP), for optimal bone ingrowth (osteointegration).
- Cobalt Chromium alloy (CoCr).
- Anatomical conical shape.
- 7 sizes right and 7 sizes left components.



Reference	Description
HINTEGRA® - Talar Component with Pegs - Right	
301110	HINTEGRA® talar component with pegs-right - size 0
301111	HINTEGRA® talar component with pegs-right - size 1
301112	HINTEGRA® talar component with pegs-right - size 2
301113	HINTEGRA® talar component with pegs-right - size 3
301114	HINTEGRA® talar component with pegs-right - size 4
301115	HINTEGRA® talar component with pegs-right - size 5
301116	HINTEGRA® talar component with pegs-right - size 6
HINTEGRA® - Talar Component with Pegs - Left	
302110	HINTEGRA® talar component with pegs-left - size 0
302111	HINTEGRA® talar component with pegs-left - size 1
302112	HINTEGRA® talar component with pegs-left - size 2
302113	HINTEGRA® talar component with pegs-left - size 3
302114	HINTEGRA® talar component with pegs-left - size 4
302115	HINTEGRA® talar component with pegs-left - size 5
302116	HINTEGRA® talar component with pegs-left - size 6

HINTEGRA® Total Ankle Prosthesis – (Optional) Tibial cortical screw – Primary Surgery


- Stainless steel M30NW.
- Optionally to be put only with tibial components.



Reference	Description
303328S	HINTEGRA® cortical screw - Dia. 3.5 mm x L. 28 mm - tibia - size 0
303330S	HINTEGRA® cortical screw - Dia. 3.5 mm x L. 30 mm - size 1
303334S	HINTEGRA® cortical screw - Dia. 3.5 mm x L. 34 mm - size 2
303338S	HINTEGRA® cortical screw - Dia. 3.5 mm x L. 38 mm - size 3
303340S	HINTEGRA® cortical screw - Dia. 3.5 mm x L. 40 mm - size 4
303342S	HINTEGRA® cortical screw - Dia. 3.5 mm x L. 42 mm - size 5 & 6

 250
 240
 230
 220
 210
 200
 190
 180
 170
 160
 150
 140
 130
 120
 110
 100
 90
 80
 70
 60
 50
 40
 30
 20
 10
 0
 MILLIMETERS

HINTEGRA® Total Ankle Prosthesis Associated Instruments for Primary Surgery

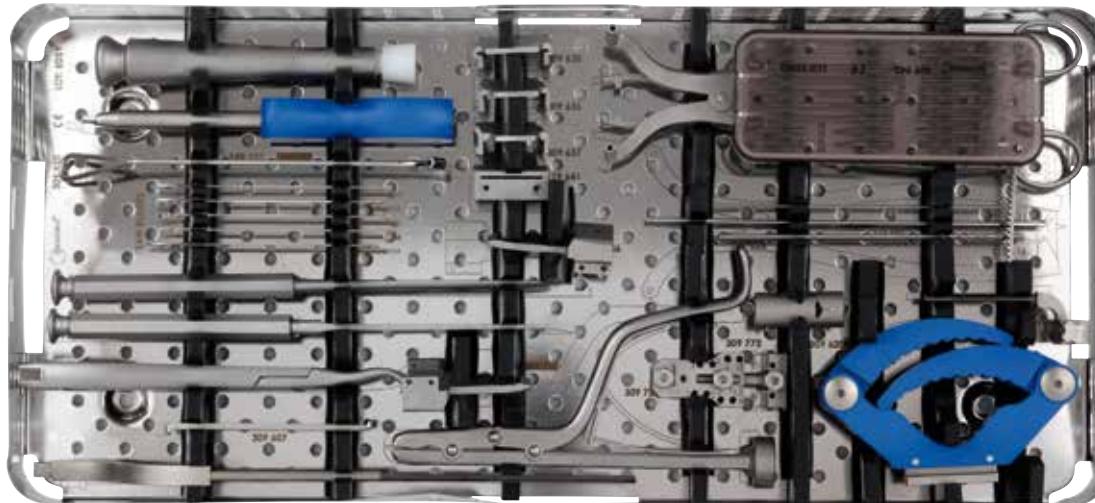

Generic base
(upper tray)



Trial tray



Talar base

HINTEGRA® Total Ankle Prosthesis Associated Instruments for Primary Surgery

Instruments for LOWER TRAY

Talar Base	
309300	Drilling guide talus - Size 0
309301	Drilling guide talus - Size 1
309302	Drilling guide talus - Size 2
309303	Drilling guide talus - Size 3
309304	Drilling guide talus - Size 4
309305	Drilling guide talus - Size 5
309306	Drilling guide talus - Size 6
309360	Tal. cut. guide-Right - Size 0
309361	Tal. cut. guide-Right - Size 1
309362	Tal. cut. guide-Right - Size 2
309363	Tal. cut. guide-Right - Size 3
309364	Tal. cut. guide-Right - Size 4
309365	Tal. cut. guide-Right - Size 5
309366	Tal. cut. guide-Right - Size 6
309370	Tal. cut. guide-Left - Size 0
309371	Tal. cut. guide-Left - Size 1
309372	Tal. cut. guide-Left - Size 2
309373	Tal. cut. guide-Left - Size 3
309374	Tal. cut. guide-Left - Size 4
309375	Tal. cut. guide-Left - Size 5
309376	Tal. cut. guide-Left - Size 6
309601	Screwdriver tibial screws
309608	Spacer h 12 mm
119609	Talar impactor
119641	Cutting guide tibial revision
309200	Reamer talar dia. 6 mm
309309	Peg drill talus - dia. 4.5 mm
309697	Holder trial talar implant
309699	Impactor trial talar implant

Trial Tray

HINTEGRA® Tibial Trial-Right	
119646	Tibial Trial-Right - Size 0
119690	Tibial Trial-Right - Size 1
119691	Tibial Trial-Right - Size 2
119692	Tibial Trial-Right - Size 3
119693	Tibial Trial-Right - Size 4
119694	Tibial Trial-Right - Size 5
119778	Tibial Trial-Right - Size 6
HINTEGRA® Tibial Trial-Left	
119647	Tibial Trial-Left - Size 0
119695	Tibial Trial-Left - Size 1
119696	Tibial Trial-Left - Size 2
119697	Tibial Trial-Left - Size 3
119698	Tibial Trial-Left - Size 4
119699	Tibial Trial-Left - Size 5
119779	Tibial Trial-Left - Size 6
HINTEGRA® Talar Trial-Right	
309680	Talar Trial-Right - Size 0
309681	Talar Trial-Right - Size 1
309682	Talar Trial-Right - Size 2
309683	Talar Trial-Right - Size 3
309684	Talar Trial-Right - Size 4
309685	Talar Trial-Right - Size 5
309686	Talar Trial-Right - Size 6
HINTEGRA® Talar Trial-Left	
309690	Talar Trial-Left - Size 0
309691	Talar Trial-Left - Size 1
309692	Talar Trial-Left - Size 2
309693	Talar Trial-Left - Size 3
309694	Talar Trial-Left - Size 4
309695	Talar Trial-Left - Size 5
309696	Talar Trial-Left - Size 6
HINTEGRA® Trial inlay	
119665	Trial inlay - thickness 5mm
119666	Trial inlay - thickness 6mm
119667	Trial inlay - thickness 7mm
119669	Trial inlay - thickness 9 mm

Sterilization container

309900 HINTEGRA® Container (Upper + Lower) including:			
309902	Stainless steel base upper, including:	309904	Stainless steel base lower, including:
309920	Generic base	309960	Talar base
309940	Pins insert	309980	Thermo insert trial implants
309942	Lid pins insert	309970	Lid trial implants
		996350	Lid
		119909	Silicone wedge

HINTEGRA® Total Ankle Prosthesis – Flat Cut – Revision Surgery

- Double coating: Porous Titanium & Hydroxyapatite (Ti and HAP), for optimal bone ingrowth (osteointegration).



HINTEGRA® Total Ankle Prosthesis Flat Cut – Tibial Component – Revision Surgery

- Double coating: Porous Titanium & Hydroxyapatite (Ti and HAP), for optimal bone ingrowth (osteointegration).
- Two thicknesses: 8 and 12 mm.



Reference	Description	Reference	Description
HINTEGRA® - revision tibial component - right - 8 mm			HINTEGRA® - revision tibial component - right - 12 mm
301222	HINTEGRA® revision tibial component-right-8 mm - size 2	301232	HINTEGRA® revision tibial component-right-12 mm - size 2
301223	HINTEGRA® revision tibial component-right-8 mm - size 3	301233	HINTEGRA® revision tibial component-right-12 mm - size 3
301224	HINTEGRA® revision tibial component-right-8 mm - size 4	301234	HINTEGRA® revision tibial component-right-12 mm - size 4
301225	HINTEGRA® revision tibial component-right-8 mm - size 5	301235	HINTEGRA® revision tibial component-right-12 mm - size 5
HINTEGRA® - revision tibial component - left - 8 mm			HINTEGRA® - revision tibial component - left - 12 mm
302222	HINTEGRA® revision tibial component-left-8 mm - size 2	302232	HINTEGRA® revision tibial component-left-12 mm - size 2
302223	HINTEGRA® revision tibial component-left-8 mm - size 3	302233	HINTEGRA® revision tibial component-left-12 mm - size 3
302224	HINTEGRA® revision tibial component-left-8 mm - size 4	302234	HINTEGRA® revision tibial component-left-12 mm - size 4
302225	HINTEGRA® revision tibial component-left-8 mm - size 5	302235	HINTEGRA® revision tibial component-left-12 mm - size 5

HINTEGRA® Total Ankle Prosthesis Flat Cut – Talar Component – Revision Surgery / Flat Talus

- For flat talus and revision surgeries.
- Double coating: Porous Titanium & Hydroxyapatite (Ti and HAP), for optimal bone ingrowth (osteointegration).



Reference	Description	Reference	Description
HINTEGRA® - flat cut talar component - right			HINTEGRA® - flat cut talar component - left
301121	HINTEGRA® revision talar component-right - size 1	302121	HINTEGRA® revision talar component-left - size 1
301122	HINTEGRA® revision talar component-right - size 2	302122	HINTEGRA® revision talar component-left - size 2
301123	HINTEGRA® revision talar component-right - size 3	302123	HINTEGRA® revision talar component-left - size 3
301124	HINTEGRA® revision talar component-right - size 4	302124	HINTEGRA® revision talar component-left - size 4
301125	HINTEGRA® revision talar component-right - size 5	302125	HINTEGRA® revision talar component-left - size 5

HINTEGRA® Total Ankle Prosthesis – Cortical screw

- Stainless steel: M30NW.
- Sterile.



Reference	Description
303312S	HINTEGRA® cortical screw - dia. 3.5 mm x l. 12 mm - talus
303316S	HINTEGRA® cortical screw - dia. 3.5 mm x l. 16 mm - talus
303320S	HINTEGRA® cortical screw - dia. 3.5 mm x l. 20 mm - talus
303334S	HINTEGRA® cortical screw - dia. 3.5 mm x l. 34 mm - tibia - size 2
303338S	HINTEGRA® cortical screw - dia. 3.5 mm x l. 38 mm - tibia - size 3
303340S	HINTEGRA® cortical screw - dia. 3.5 mm x l. 40 mm - tibia - size 4
303342S	HINTEGRA® cortical screw - dia. 3.5 mm x l. 42 mm - tibia - size 5 & 6

HINTEGRA® Total Ankle Prosthesis – PE Inlay – Revision Surgery (See page 19 for product references.)

Size of the PE inlay has to be the same as the talar component.


**HINTEGRA® Total Ankle Prosthesis – Flat Cut
Instruments for Revision Surgery**
Instruments

119790	FC Talar Trial for Drilling-Right - Size 1
119791	FC Talar Trial for Drilling-Right - Size 2
119792	FC Talar Trial for Drilling-Right - Size 3
119793	FC Talar Trial for Drilling-Right - Size 4
119794	FC Talar Trial for Drilling-Right - Size 5

119657 Drill dia. 4.5 mm x L. 22 mm

119659 FC Talar trial for drilling Impactor

119795 FC Talar Trial for Drilling-Left - Size 1

119796 FC Talar Trial for Drilling-Left - Size 2

119797 FC Talar Trial for Drilling-Left - Size 3

119798 FC Talar Trial for Drilling-Left - Size 4

119799 FC Talar Trial for Drilling-Left - Size 5

119631 FC Spacer 4 mm for revision Tibial Component 8 mm

119632 FC Spacer 8 mm for revision Tibial Component 12 mm

119757 FC spacer

119760 FC Talar Cutting Guide-Right - Size 1

119761 FC Talar Cutting Guide-Right - Size 2

119762 FC Talar Cutting Guide-Right - Size 3

119763 FC Talar Cutting Guide-Right - Size 4

119764 FC Talar Cutting Guide-Right - Size 5

119765 FC Talar Cutting Guide-Left - Size 1

119766 FC Talar Cutting Guide-Left - Size 2

119767 FC Talar Cutting Guide-Left - Size 3

119768 FC Talar Cutting Guide-Left - Size 4


119769 FC Talar Cutting Guide-Left - Size 5

309 708 Tibial depth gauge for tibial component 8 mm

309712 Tibial depth gauge for tibial component 12 mm

Sterilization container

119965	HINTEGRA® FC revision container includes:
119978	Container pocket
119966	HINTEGRA® FC container base
119967	Lid for HINTEGRA® FC container base

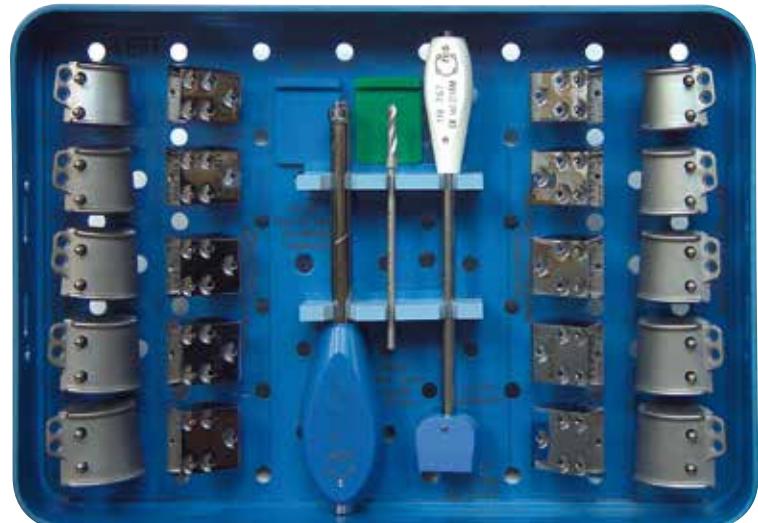

HINTEGRA® Sensitive Total Ankle Prosthesis – Primary Surgery

The Hintegra® Sensitive Total Ankle Prosthesis is also a three component design specially made for allergic patients.

- Materials:
 - > Talar & Tibial components:
 - » Cobalt Chromium alloy (CoCr) with Titanium Nitride (TiN) coating.
 - > PE inlay:
 - » Polyethylene (UHMWPE).



HINTEGRA® Sensitive Total Ankle Prosthesis – Tibial Component – Primary Surgery

- Anatomical shape for minimal contact stress to the bone.
- Cobalt Chromium alloy (CoCr) with Titanium Nitride (TiN) coating.
- 6 right and 6 left components.

Reference	Description
HINTEGRA® sensitive - tibial component - right	
351251	HINTEGRA® sensitive - tibia-right - size 1
351252	HINTEGRA® sensitive - tibia-right - size 2
351253	HINTEGRA® sensitive - tibia-right - size 3
351254	HINTEGRA® sensitive - tibia-right - size 4
351255	HINTEGRA® sensitive - tibia-right - size 5
351256	HINTEGRA® sensitive - tibia-right - size 6
HINTEGRA® sensitive - tibial component - left	
352251	HINTEGRA® sensitive - tibia-left - size 1
352252	HINTEGRA® sensitive - tibia-left - size 2
352253	HINTEGRA® sensitive - tibia-left - size 3
352254	HINTEGRA® sensitive - tibia-left - size 4
352255	HINTEGRA® sensitive - tibia-left - size 5
352256	HINTEGRA® sensitive - tibia-left - size 6



HINTEGRA® Sensitive Total Ankle Prosthesis – Talar component with Pegs – Primary Surgery

- Cobalt Chromium alloy (CoCr) with Titanium Nitride (TiN) coating.
- Anatomical conical shape.
- 5 sizes and 5 left components.

Reference	Description
HINTEGRA® - talar component with pegs - right	
351152	HINTEGRA® sensitive - talus -right - size 2
351153	HINTEGRA® sensitive - talus -right - size 3
351154	HINTEGRA® sensitive - talus -right - size 4
351155	HINTEGRA® sensitive - talus -right - size 5
351156	HINTEGRA® sensitive - talus -right - size 6
HINTEGRA® - talar component with pegs - left	
352152	HINTEGRA® sensitive - talus-left - size 2
352153	HINTEGRA® sensitive - talus-left - size 3
352154	HINTEGRA® sensitive - talus-left - size 4
352155	HINTEGRA® sensitive - talus-left - size 5
352156	HINTEGRA® sensitive - talus-left - size 6



HINTEGRA® Sensitive Total Ankle Prosthesis – PE Inlay (See page 45 for product references.)

- HINTEGRA® PE inlays are “sensitive compatible” since metallic rods are made of titanium Alloy (TA6V).
- Size of the PE inlay has to be the same as the talar component.



HINTEGRA® Sensitive Total Ankle Prosthesis – (Optional) Tibial cortical screw

- Titanium alloy (TA6V).
- Optionally to be put only with tibial components.

Reference	Description
303530S	Cortical Screw Ti - Dia. 3.5 mm x L. 30 mm - Tibia - Size 1
303534S	Cortical Screw Ti - Dia. 3.5 mm x L. 34 mm - Tibia - Size 2
303538S	Cortical Screw Ti - Dia. 3.5 mm x L. 38 mm - Tibia - Size 3
303540S	Cortical Screw Ti - Dia. 3.5 mm x L. 40 mm - Tibia - Size 4
303542S	Cortical Screw Ti - Dia. 3.5 mm x L. 42 mm - Tibia - Size 5 & 6



HINTEGRA® Sensitive Total Ankle Prosthesis – Flat Cut – Revision Surgery

The HINTEGRA® Sensitive Total Ankle Prosthesis is also a three component design specially made for allergic patients.

- Materials:
 - Talar & Tibial components:
 - Cobalt Chromium alloy (CoCr) with Titanium Nitride (TiN) coating.
 - PE inlay:
 - Polyethylene (UHMWPE).



HINTEGRA® Sensitive Total Ankle Prosthesis – Flat Cut – Tibial Component – Revision Surgery

- Anatomical shape for minimal contact stress to the bone.
- Cobalt Chromium alloy (CoCr) with Titanium Nitride (TiN) coating.
- 4 right and 4 left components.

Reference	Description	Reference	Description
HINTEGRA® – Revision Tibial Component - Right - 8 mm		HINTEGRA® – Revision Tibial Component - Right - 12 mm	
351522	HINTEGRA® sensitive FC - tibia-right 8 mm - size 2	351532	HINTEGRA® sensitive FC - tibia-right 12 mm - size 2
351523	HINTEGRA® sensitive FC - tibia-right 8 mm - size 3	351533	HINTEGRA® sensitive FC - tibia-right 12 mm - size 3
351524	HINTEGRA® sensitive FC - tibia-right 8 mm - size 4	351534	HINTEGRA® sensitive FC - tibia-right 12 mm - size 4
351525	HINTEGRA® sensitive FC - tibia-right 8 mm - size 5	351535	HINTEGRA® sensitive FC - tibia-right 12 mm - size 5
HINTEGRA® – Revision Tibial Component - Left - 8 mm		HINTEGRA® – Revision Tibial Component - Left - 12 mm	
352522	HINTEGRA® sensitive FC - tibia-left 8 mm - size 2	352532	HINTEGRA® sensitive FC - tibia-left 12 mm - size 2
352523	HINTEGRA® sensitive FC - tibia-left 8 mm - size 3	352533	HINTEGRA® sensitive FC - tibia-left 12 mm - size 3
352524	HINTEGRA® sensitive FC - tibia-left 8 mm - size 4	352534	HINTEGRA® sensitive FC - tibia-left 12 mm - size 4
352525	HINTEGRA® sensitive FC - tibia-left 8 mm - size 5	352535	HINTEGRA® sensitive FC - tibia-left 12 mm - size 5



HINTEGRA® Sensitive Total Ankle Prosthesis – Flat Cut

Talar component with Pegs – Revision Surgery / Flat talus

- Cobalt Chromium alloy (CoCr) with Titanium Nitride (TiN) coating.
- 4 right and 4 left components.

Reference	Description
HINTEGRA® - Talar Component with Pegs - Right	
351512	HINTEGRA® sensitive FC - talus-right - size 2
351513	HINTEGRA® sensitive FC - talus-right - size 3
351514	HINTEGRA® sensitive FC - talus-right - size 4
351515	HINTEGRA® sensitive FC - talus-right - size 5
HINTEGRA® - Talar Component with Pegs - Left	
352512	HINTEGRA® sensitive FC - talus-left - size 2
352513	HINTEGRA® sensitive FC - talus-left - size 3
352514	HINTEGRA® sensitive FC - talus-left - size 4
352515	HINTEGRA® sensitive FC - talus-left - size 5



HINTEGRA® Sensitive Total Ankle Prosthesis – PE Inlay

(See page 45 for product references.)

- HINTEGRA® PE inlays are “sensitive compatible” since metallic rods are made of titanium Alloy (TA6V).
- Size of the PE inlay has to be the same as the talar component.



HINTEGRA® Sensitive Total Ankle Prosthesis – Flat Cut – Cortical screw

Titanium alloy (TA6V).

Reference	Description
303512S	Cortical Screw Ti - dia.3.5 x L. 12 mm - Talus
303516S	Cortical Screw Ti - dia.3.5 x L. 16 mm - Talus
303520S	Cortical Screw Ti - dia.3.5 x L. 20 mm - Talus
303534S	Cortical Screw Ti - dia. 3.5 x L. 34 mm - Tibia - Size 2
303538S	Cortical Screw Ti - dia. 3.5 x L. 38 mm - Tibia - Size 3
303540S	Cortical Screw Ti - dia. 3.5 x L. 40 mm - Tibia - Size 4
303542S	Cortical Screw Ti - dia. 3.5 x L. 42 mm - Tibia - Size 5



PANTA® / PANTA® XL Arthrodesis Nail

The PANTA® Nail is intended for use in tibiotalocalcaneal arthrodesis and treatment of trauma of the hindfoot and distal tibia.

- Cannulated Titanium Nail.
- Radio-transparent instrumentation system to apply compression.
- Multi-axial fixation:
 - > Oblique antero-posterior calcaneal screws.
 - > Medio-lateral tibial screws.
- 2 kind of screws:
 - > Oblique antero-posterior calcaneal screws.
 - » fully threaded
 - » partially threaded
- 5 mm diameter Titanium screw.
- Screw lengths: 20 to 110 mm.
- Material of the nail, the screws and the end cap: Titanium alloy TA6V.

PANTA® Nails (sterile)

Reference	Dia. - length
500050	Dia. 10 mm - L. 150 mm
500080	Dia. 10 mm - L. 180 mm
500150	Dia. 11 mm - L. 150 mm
500180	Dia. 11 mm - L. 180 mm
500250	Dia. 12 mm - L. 150 mm
500280	Dia. 12 mm - L. 180 mm
500350	Dia. 13 mm - L. 150 mm
500380	Dia. 13 mm - L. 180 mm

PANTA® XL Nails (sterile)

To be used only with Partially threaded Screws

Reference	Dia. - length
510111	Dia. 11mm - L 210 mm
510141	Dia. 11mm - L 240 mm
510211	Dia. 12 mm - L 210 mm
510241	Dia. 12 mm - L 240 mm
510311	Dia. 13mm - L 210 mm
510341	Dia. 13mm - L 240 mm

End cap (sterile)

Reference	Description
500001	End cap
510005	Locking end cap



PANTA[®] Arthrodesis Nail – Fully threaded screws dia. 5 mm (not for use with PANTA[®] XL Arthrodesis Nail)

Reference	Length
501020	L. 20 mm
501022	L. 22.5 mm
501025	L. 25 mm
501027	L. 27.5 mm
501030	L. 30 mm
501035	L. 35 mm
501040	L. 40 mm
501045	L. 45 mm
501050	L. 50 mm
501055	L. 55 mm
501060	L. 60 mm
501065	L. 65 mm
501070	L. 70 mm
501075	L. 75 mm
501080	L. 80 mm
501085	L. 85 mm
501090	L. 90 mm
501095	L. 95 mm
501100	L. 100 mm
501105	L. 105 mm
501110	L. 110 mm


PANTA[®] / PANTA[®] XL Arthrodesis Nail – Partially threaded lag screws dia. 5 mm

Reference	Length
511020	L. 20 mm
511022	L. 22.5 mm
511025	L. 25 mm
511027	L. 27.5 mm
511030	L. 30 mm
511035	L. 35 mm
511040	L. 40 mm
511045	L. 45 mm
511050	L. 50 mm
511055	L. 55 mm
511060	L. 60 mm
511065	L. 65 mm
511070	L. 70 mm
511075	L. 75 mm
511080	L. 80 mm
511085	L. 85 mm
511090	L. 90 mm
511095	L. 95 mm
511100	L. 100 mm
511105	L. 105 mm
511110	L. 110 mm



PANTA® Arthrodesis Nail – Instruments

Reference	Description
519003	Drill dia. 4.3 mm for Calcaneum Screws
519004	Drill dia. 4.3 mm for Tibial Screws
519005	Drill dia. 5.0 mm – AO Attachment
519006	Long drill for calcaneus screws dia. 4.3 mm
519007	Cannulated Drill dia. 7.0 mm
519009	Cannulated Drill dia. 9.0 mm
519011	Reamer dia. 11 mm
519012	Reamer dia. 12 mm
519013	Reamer dia. 13 mm
519014	Reamer dia. 10.5 mm
519015	Reamer dia. 11.5 mm
519016	Reamer dia. 12.5 mm
519017	Reamer dia. 13.5 mm
519021	T Handle AO Attachment
519028	Internal Protecting Sleeve dia. 3.2 mm
519029	Central Internal Protecting Sleeve dia. 9.0 mm
519030	External Protecting Sleeve
519032	Pin dia. 3.2 mm x L. 400 mm
519040	Trocard Awl
519110	Support Device
519120	Nail Fixation Axis
519121	Toothed Wheel
519131	Threaded Axis
519130	Compression Device
519133	Teflon Ring
519135	Compression Wheel
519160	Depth Gauge
519175	Compression Rod
519179	Short Drill Guide dia. 4.3 mm L. 70 mm
519180	Long Drill Guide dia. 4.3 mm L. 120 mm
519181	Drill Guide dia. 5.0 mm
519184	Short Drill Guide dia. 7.0 mm L. 70 mm
519185	Drill Guide dia. 7.0 mm L. 120 mm
519290	Hexagonal screwdriver tip dia. 3.5 mm
519295	Hexagonal screwdriver dia. 3.5 mm
539015	Tap dia. 6.5 mm

PANTA® – Sterilization Container

519920	PANTA® sterilization container including:
519910	PANTA® base
519911	PANTA® Insert
519920	Lid
119909	Silicone wedge

PANTA® – Optional Instruments



519010	Reamer dia. 10 mm
519020	Quick Coupling AO
519002	Short drill for calcaneus screws used with medium drill guide dia. 4.3 mm
519008	Long drill for calcaneus screws used with medium drill guide dia. 4.3 mm
519034(S)	Guide wire dia. 3.2 mm, L. 600 mm (sterile upon request)
519178	Medium drill guide dia. 4.3 mm
519183	Medium soft tissue protector dia. 7 mm

PANTA® XL – Associated Instruments (optional)

539020	Conical reamer dia. 10.5 mm
539021	Conical reamer dia. 11.5 mm
539022	Conical reamer dia. 12.5 mm
539023	Conical reamer dia. 13.5 mm
519912	Reamer holder



(S) means available in sterile and non sterile

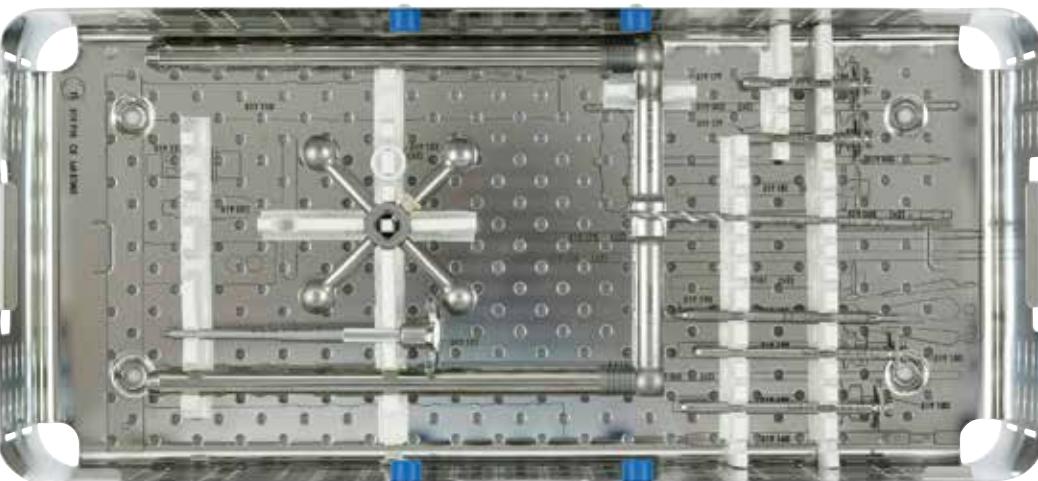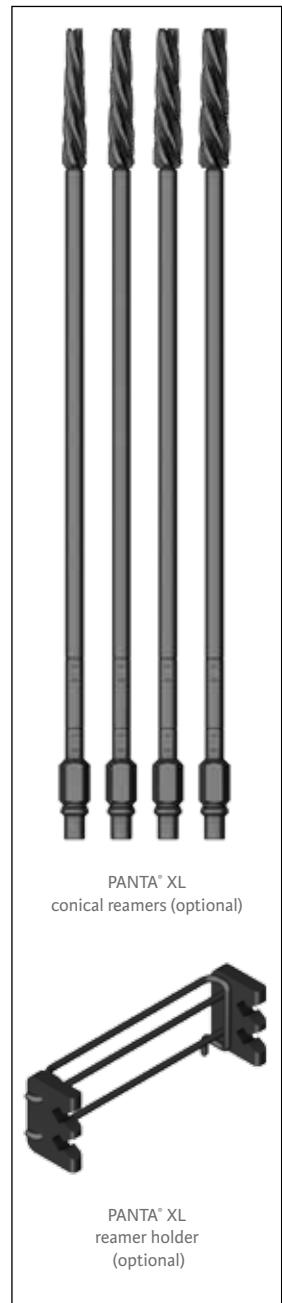PANTA[®] Arthrodesis Nail - Associated Instruments

250
240
230
220
210
200
190
180
170
160
150
140
130
120
110
100
90
80
70
60
50
40
30
20
10
0
MILLIMETERS

PANTA® Removal Set

Reference	Description
519209	Sliding hammer
519210	Handle extractor
309645	Screwdriver Hex dia.3.5 mm
119552	External protection sleeve dia.6.5 mm
Sterilization container	
519950	PANTA® Removal sterilization container
119909	Silicone wedge
519951	Basis
996100	Lid



ADVANSYS[®] TTC Fusion Plate

The TTC Plates are intended for arthrodesis of the ankle joint and calcanea, osteotomies, fusions and replantations of small bones in the ankle and distal tibia.

- 4 sizes of implants
 - > 4 right & 4 left plates (in 6,7,8,9 holes configurations).
- Screw dia.4.5 mm for fixation of the tibia and talus – Length 14 mm to 65 mm.
- Screw dia.6.5 mm for fixation of the calcaneus – Length 20 mm to 65 mm.
- Lock-screws for 4.5 mm dia. screws.
- Lock-screws for 6.5 mm dia. screws.
- Material:
 - > Plate: Stainless Steel 316LVM.
 - > Screw: Titanium TA6V.



Advansys[®] TTC Fusion Plate

Reference	Description
181001S	ADVANSYS [®] TTCP Right-6 holes
181002S	ADVANSYS [®] TTCP Right-8 holes
181003S	ADVANSYS [®] TTCP Right-7 holes
181004S	ADVANSYS [®] TTCP Right-9 holes
181011S	ADVANSYS [®] TTCP Left-6 holes
181012S	ADVANSYS [®] TTCP Left-8 holes
181013S	ADVANSYS [®] TTCP Left-7 holes
181014S	ADVANSYS [®] TTCP Left-9 holes



Surfix[®] Locking screw
Sterile Titanium dia. 4.5 mm + lock-screw

Reference	Length
285414S	L. 14 mm
285416S	L. 16 mm
285418S	L. 18 mm
285420S	L. 20 mm
285422S	L. 22 mm
285424S	L. 24 mm
285426S	L. 26 mm
285428S	L. 28 mm
285430S	L. 30 mm
285435S	L. 35 mm
285440S	L. 40 mm
285445S	L. 45 mm
285450S	L. 50 mm
285455S	L. 55 mm
285460S	L. 60 mm
285465S	L. 65 mm
185400S	SURFIX [®] Lock Screw dia. 4.5 mm



Surfix[®] Locking screw
Sterile Titanium dia. 6.5 mm + lock-screw

Reference	Length
285620S	L. 20 mm
285625S	L. 25 mm
285630S	L. 30 mm
285635S	L. 35 mm
285640S	L. 40 mm
285645S	L. 45 mm
285650S	L. 50 mm
285655S	L. 55 mm
285660S	L. 60 mm
285665S	L. 65 mm
185600S	SURFIX [®] lock Screw dia. 6.5 mm

Optional instrument

Reference	Description
MA3511	Surfix [®] screw extractor 3.5 mm

250
240
230
220
210
200
190
180
170
160
150
140
130
120
110
100
90
80
70
60
50
40
30
20
10
MILLIMETERS

ADVANSYS[®] TTC Fusion Plate Instruments


Reference	Description
219845	Screwdriver hexa 2.5 x L. 191 mm
219865	Screwdriver hexa dia.3.5 x L. 230 mm
219445	AO Screwdriver tip hexa dia.2.5 x L. 76 mm
219465	AO Screwdriver tip hexa dia.3.5 x L. 76 mm
219645	Drilling guide dia.3.0 mm
219665	Drilling guide dia.3.5 mm
219545	AO Drill dia.3.0 x L. 190 mm
219565	Drill dia.3.5 x L. 200 mm
219900	Compression forceps L. 260 mm
219765	Bending forceps L. 193 - hole dia.6.5 mm
219345	Depth gauge hole dia.4.5 mm
219365	Depth gauge hole dia.6.5 mm
115116	K-Wire dia.1.6 x L. 150 mm
115425	K-Wire dia.2.5 x L. 200 mm
169001	TTCP trial implant 6 holes
169002	TTCP trial implant 8 holes
169003	TTCP trial implant 7 holes
169004	TTCP trial implant 9 holes

Sterilization container

169101	ADVANSYS [®] Hindfoot sterilization container including:
169111	Base
996200	Lid
169104	Cylinder
169105	TTCP trial implant module
119909	Silicone wedge

Optional instrument

Reference	Description
MA3511	Surfix [®] screw extractor 3.5 mm

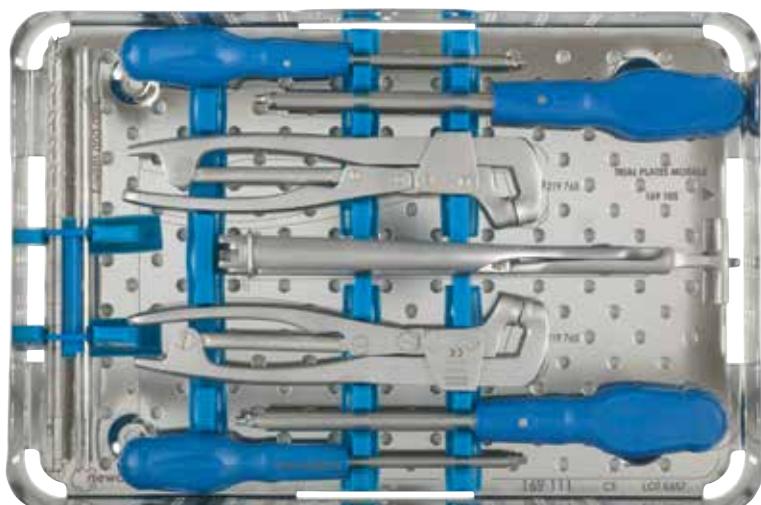



TIBIAXYS® Ankle Arthrodesis Plating System

TIBIAXYS® Distal Tibia and Fibula Osteotomy Plating Systems

The TIBIAXYS® Plates are intended for fixation of arthrodesis osteotomies and fractures of ankle joint, distal tibia and fibula.

- Each plate is anatomically contoured and available in 1 size.
- 2 systems of 2 anterior plates for ankle fusion (green left and blue right systems, including 1 antero-medial and 1 antero-lateral plates).
- 3 different plates for distal tibia osteotomies (medial plate, left lateral / right medial anterior plate, left medial/ right lateral anterior plate).
- 2 different plates for fibula osteotomies (4 and 6 holes).

- dia. 3.5 mm Surfix® or Surfix®-Alpha screws and lock-screws.
- dia. 4.0 mm cortical screws (only for 1 hole in each plate for the ankle fusion).
- Material:
 - > Plates: Titanium alloy TA6V.
 - > Surfix® and Surfix®-Alpha screws and lock-screws: Titanium alloy TA6V.
 - > Cortical screws: Titanium alloy TA6V.

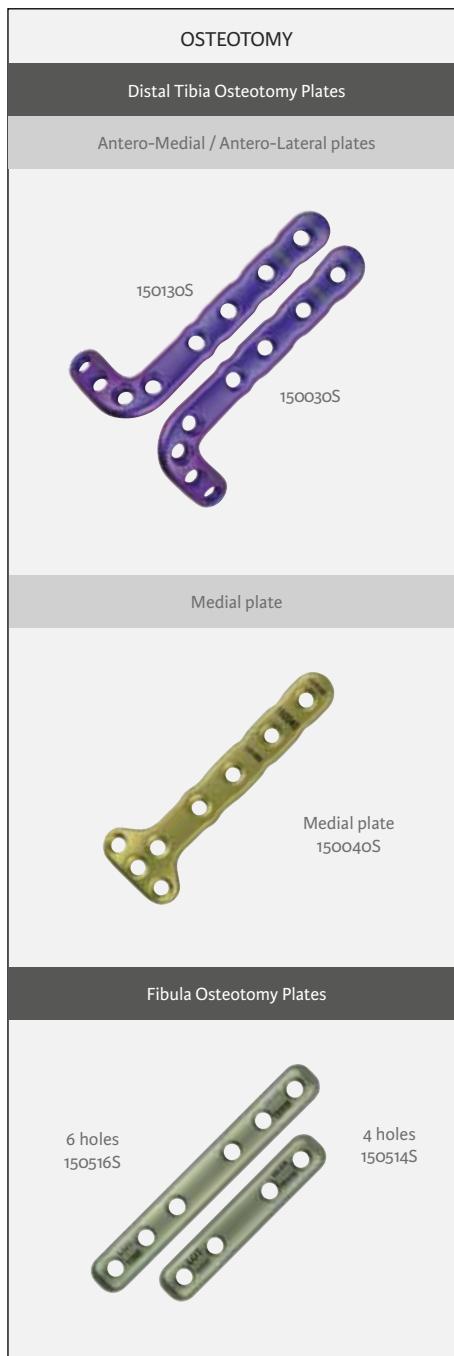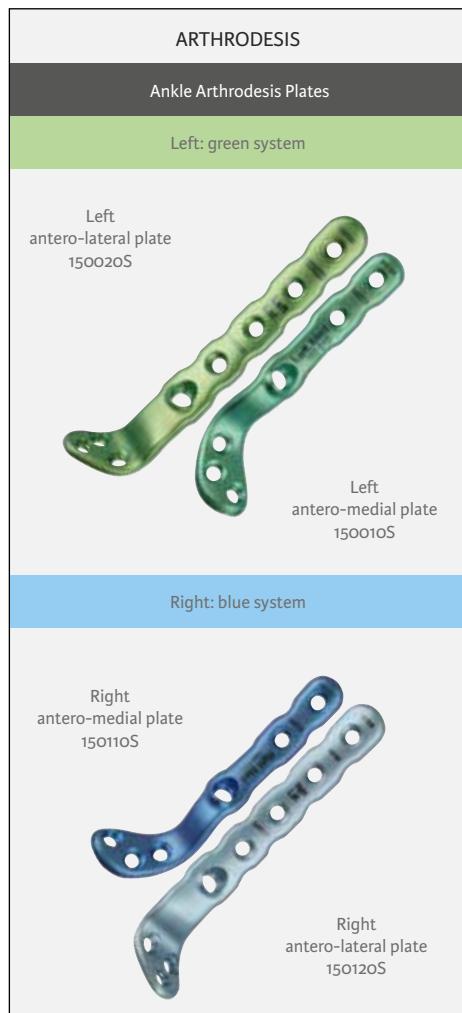

Reference	Description
150010S	TIBIAXYS® Arthrodesis Plate / Left antero-medial
150020S	TIBIAXYS® Arthrodesis Plate / Left antero-lateral
150110S	TIBIAXYS® Arthrodesis Plate / right antero-medial
150120S	TIBIAXYS® Arthrodesis Plate / right antero-lateral

Reference	Description
150030S	TIBIAXYS® Osteotomy Plate / Lateral-right / Medial-left
150130S	TIBIAXYS® Osteotomy Plate / Medial-right / Lateral-left
150040S	TIBIAXYS® Osteotomy Plate / Medial

Reference	Description
150514S	TIBIAXYS® Fibula Osteotomy Plate 4 holes
150516S	TIBIAXYS® Fibula Osteotomy Plate 6 holes

Optional instrument

Reference	Description
MA3511	Surfix® screw extractor 3.5 mm

TIBIAXYS® Ankle Arthrodesis Plating System
TIBIAXYS® Distal Tibia and Fibula Osteotomy Plating Systems



Surfix®-Alpha variable angle locking screws – Sterile Titanium dia. 3.5 mm + lock-screw

Reference	Length
295310S	L. 10 mm
295312S	L. 12 mm
295314S	L. 14 mm
295316S	L. 16 mm
295318S	L. 18 mm
295320S	L. 20 mm
295322S	L. 22 mm
295324S	L. 24 mm
295326S	L. 26 mm
295328S	L. 28 mm
295330S	L. 30 mm
295332S	L. 32 mm
295334S	L. 34 mm
295336S	L. 36 mm
295338S	L. 38 mm
295340S	L. 40 mm
295344S	L. 44 mm
295348S	L. 48 mm
295350S	L. 50 mm
195300S	Lock-screw dia. 3.5 mm



**Surfix® Locking screws
Sterile Titanium dia. 3.5 mm + lock-screw**

Reference	Length
285310S	L. 10 mm
285312S	L. 12 mm
285314S	L. 14 mm
285316S	L. 16 mm
285318S	L. 18 mm
285320S	L. 20 mm
285322S	L. 22 mm
285324S	L. 24 mm
285326S	L. 26 mm
285328S	L. 28 mm
285330S	L. 30 mm
285332S	L. 32 mm
285334S	L. 34 mm
285336S	L. 36 mm
285338S	L. 38 mm
285340S	L. 40 mm
285344S	L. 44 mm
285348S	L. 48 mm
285350S	L. 50 mm
185300S	Lock-screw dia. 3.5 mm



Sterile Titanium cortical screw dia. 4.0 mm


Reference	Length
150240S	L. 40 mm
150242S	L. 42 mm
150246S	L. 46 mm
150250S	L. 50 mm
150255S	L. 55 mm
150260S	L. 60 mm
150265S	L. 65 mm
150270S	L. 70 mm
150275S	L. 75 mm
150280S	L. 80 mm
150285S	L. 85 mm
150290S	L. 90 mm
150200S	L. 100 mm

Optional instrument

Reference	Description
MA3511	Surfix® screw extractor 3.5 mm

TIBIAXYS[®] Instruments

Reference	Description
115116	K-Wire dia.1.6 x L. 150 mm
115225	K-Wire dia.2.5 x L. 200 mm
159103	Wedge thickness 3 mm
159106	Wedge thickness 6 mm
159109	Wedge thickness 9 mm
159130	Cortical screw drilling guide dia.3.0 mm
159400	Depth gauge for dia.4.0 mm screws
159635	Compression forceps guide
159740	Compression forceps screw dia.4.0 x L. 40 mm
159755	Compression forceps screw dia.4.0 x L. 55 mm
159760	Compression forceps screw dia.4.0 x L. 60 mm
219035	Surfix [®] Alpha drilling guide dia.2.7 mm
219135	Screwdriver hexalobular T10
219335	Depth gauge for dia. 3.5 mm screws
219435	AO Screwdriver tip hexa 2.0 x L. 76 mm
219445	AO Screwdriver tip hexa dia.2.5 x L. 76 mm
219535	AO drill dia.2.7 x L. 125 mm
219545	AO Drill dia.3.0 x L. 190 mm
219635	Drilling guide dia.2.7 mm
219835	Screwdriver hexa dia. 2.0 x L. 180 mm
219845	Screwdriver hexa dia. 2.5 x L. 191 mm
219960	Compression forceps L. 260 mm
159010	Trial plate Left Antero-Medial
159020	Trial plate Left Antero-Lateral
159110	Trial plate Right Antero-Medial (optional)
159120	Trial plate Right Antero-Lateral (optional)
Sterilization container	
159991	Tibiаксys [®] sterilization container including
159960	Base
996200	Lid
119909	Silicone wedge
Trial container	
159010	Left medial anterior trial plate
159020	Left lateral anterior trial plate
159110	Right medial anterior trial plate
159020	Right lateral anterior trial plate
Container	
159071	Base
309942	Lid

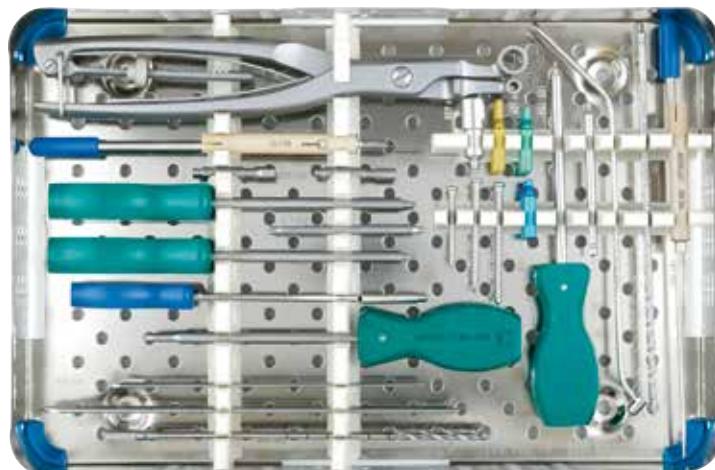

Optional instrument

Reference	Description
MA3511	Surfix [®] screw extractor 3.5 mm

ACHILLION® Minimal Invasive Achilles Tendon Suture System – Single Use

The ACHILLION® System is a method to treat acute Achilles tendon ruptures.

- Needle driver.
- Suture size: USP (3.5 metric).
- Materials:
 - > Polycarbonate.
 - > Stainless steel 316LVM.

Reference	Description
119700	ACHILLION® + 2 Needles and 1 Needle Driver



Hintermann® Distractors

Range of 4 spreading forceps.

For each of the 4 models, two pins (2.5 mm for the large model, and 1.6 or 2.5 mm diameter for the small one) are slid into the appropriate holes of the spreading forceps, and are then introduced at appropriate localisation into each of the two bone fragments to be outspread. The spreader is then distracted, and locked when the distance between the two fragments is reached.

The flexible positioning of these spreading forceps enables them not to interfere with the main procedure. These spreaders are available in two different sizes (15 cm long, or 21 cm long), and with closed or outspread arms, making them fitting many possible indication.

Hintermann® Small Distractor – 15 cm

Reference	Description
119653	Hintermann® Distractor Small open handle
119654	Hintermann® Distractor Small closed handle

Hintermann® Large Distractor – 21 cm

Reference	Description
119664	Hintermann® Distractor Big model
119651	Hintermann® Distractor Large closed handle



Hintermann® Distractor open handle



Hintermann® Distractor closed handle

Osteoguides

- Suggested use:
 - > Scarf osteotomy.
 - > Chevron osteotomy.
 - > Basal osteotomy.
 - > Arthrodesis.
 - > Wedge osteotomies (Akin...).
- Details:
 - > Hole for K-Wire: Diameter 1.0 to 1.6 mm.
 - > Knurled handle for optimal grip.
 - > Blade thickness maxi 0.8 mm.
 - > Positioning tip.

Reference	Description
229011	Longitudinal
229012	Transversal



Transversal osteotomy guide



Longitudinal osteotomy guide

K-FIX® – K-Wire End Protector

The K-Fix® pin protector is a simple system to protect patients or hospital staff from K-Wires sharp ends.

- Delivered sterile.

Reference	Length
119050	K-FIX® for K-WIRE - Dia. 0.8 mm to 2.0 mm (5 units per pack)



Weil Clamp

Reference	Length
119106	Weil Clamp

General Optional Instruments

Reference	Description
998001	Scalpel Handle N° 3
998002	Scalpel Handle N° 4
998003	Beyer Bone Rongeur Forceps
998004	Backhaus Towel Forceps
998005	Beckmann Mini Retractor
998006	Museux Forceps (14 cm)
998007	Lange- Hohmann Retractor
998008	Liston Bone Cutting Forceps
998010	Ombredanne Square Points
998011	Wolkmann Retractor
998012	Wolkmann Curette
998013	Lambotte Respiratory 12 mm
998014	Guillaume Gouge 8 mm
998015	Mac Even Hammer
998016	Redon Needle
998017	Finochieto Needle Holder 13 cm
998018	Pauwels Osteotomes 15 mm
998019	Farabeuf Retractor 12 cm
998020	Dissection Forceps (GR) 14 cm
998021	Dissection Forceps Curved 14 cm
998022	Metzenbaum Scissors
998023	Straight Scissors
998024	Mayo Scissors
998025	Leriche Forceps
998026	Verbrugge Bone Holding Forceps
998027	Poirier Gouge (14 mm)
998031	Metatarsal Head Extractor
MA3511	Surfix® screw 3.5 mm extractor
119651	Hintermann® Distractor / Large Closed Jaws
119653	Hintermann® Distractor / Small Open Jaws
119654	Hintermann® Distractor / Small Closed Jaws
119106	Weil clamp
998028	Inge Retractor
998029	Banaleck Forceps Right
998030	Banaleck Forceps Left
119909	Silicone wedge
119989	Instrument Tray



MA3511 Surfix® screw extractor 3.5 mm

Post-Operative Shoes

Reference	Description
Flat Post Operative Shoe	
999001	Small
999002	Medium
999003	Large
999004	X-Large




Reference	Description
Wedged Heel Post Operative Shoe	
999100	Size 4 to 6.5
999101	Size 7 to 8.5
999102	Size 9 to 10.5



250
240
230
220
210
200
190
180
170
160
150
140
130
120
110
100
90
80
70
60
50
40
30
20
10
MILLIMETERS

Surfix[®] Technology System

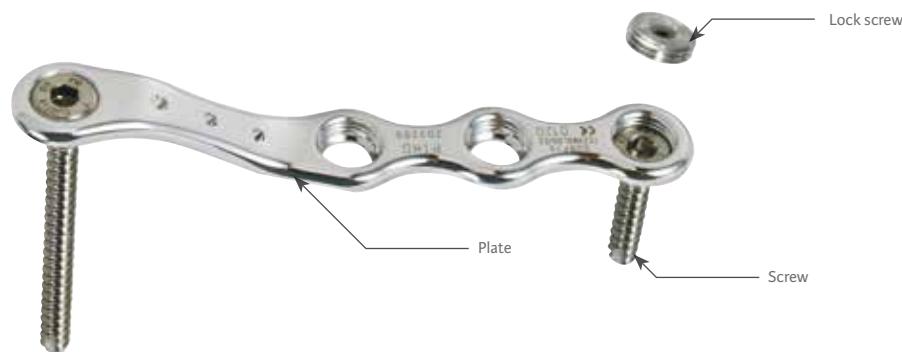


Surfix[®] Concept

Drilling:


Start with the placement of the Metacarpal Surfix[®] 2.7 mm Screw. Use the 2.0 mm Black drill through the black drill bit (It is possible to attach the drill bit to the plate).

For placement of the Surfix[®] metacarpal 3.5 mm screw to the radius. It is possible to prepare the holes with the 2.7 mm (blue) drill through blue drill bit.

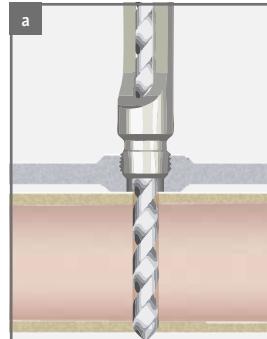

Measuring:

Measure the necessary screw length using the depth gauge (303407).

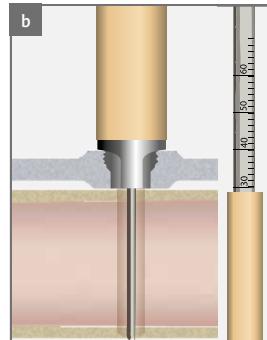


Chamfering:

Counter sink the drill hole with the Star screwdriver (303408 = Black).

Counter sink the drill hole with the 2.0 mm Hex screwdriver (303410 = Blue).

Ensure that the threaded hole is not damaged when performing the chamfering.

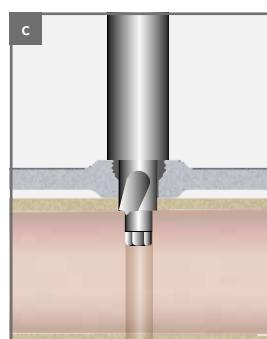


Positioning the screw:

Using the Star screwdriver (303408 = Black), insert the screw into the prepared hole until the plate is at the desired position relative to the bone.


Using the 2.0 mm Hex screwdriver (303410 = Blue), insert the screw into the prepared hole until the plate is at the desired position relative to the bone.

The screw should be fully seated in the plate. Clean the threaded hole before and after introducing the screw. Maintain co-axiality between the screw and the threaded hole.

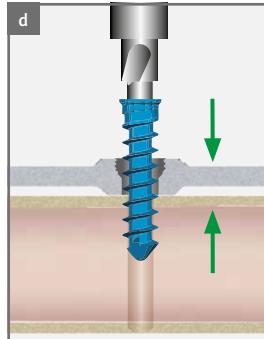


Positioning the lock-screw:

Assemble the lock-screw to the screwdriver. The lock-screw should be inserted after each screw, and before preparation and insertion of the subsequent screw. This prevents potential damage to the thread.

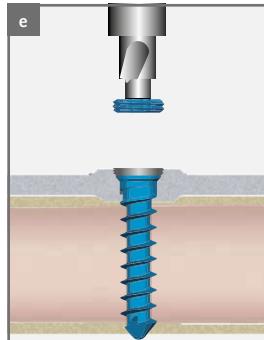

Locking:

Fully seat the lock-screw with the screwdriver. The lock-screw should be flush with the top of the plate when it is fully inserted.

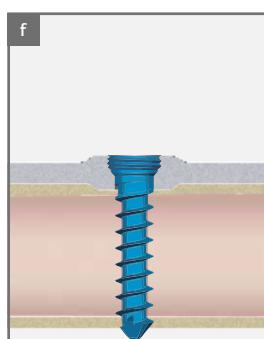



Integra®
Large Bones
Solutions
Knee and pediatric
Osteotomy plates

POF Plate

Closing Femoral Osteotomy Plate

The POF plate is indicated for distal femoral varus osteotomy and lateral gonarthrosis on genu-valgum.

- Fixation by 3 Surfix® screws into the femoral condyle for rotatory stability.
- Plate angulation adapted to the anatomy of the tibia.
- Shapeable Peg.
- Materials:
 - > Plate: Stainless steel 316L LVM Standard ISO 5832-1 & ASTM F138&139
 - > Screws and lock-screws: Titanium TA6V Standard ISO 5832-3 & ASTM F136

Reference	Description
POF	Distal Femoral Varus Osteotomy Plate



POF Plate

Associated Surfix® Screws

Surfix® Cortical bone screw

+ lock-screw diam 4.5 mm

References	Description
CC 024	Length 24 mm
CC 026	Length 26 mm
CC 028	Length 28 mm
CC 030	Length 30 mm
CC 032	Length 32 mm
CC 035	Length 35 mm
CC 040	Length 40 mm
CC 045	Length 45 mm
CC 050	Length 50 mm
CC 055	Length 55 mm
CC 060	Length 60 mm
CC 065	Length 65 mm



Surfix® Cancellous bone screw

+ lock-screw diam 6.5 mm

References	Description
SP 020	Length 20 mm
SP 025	Length 25 mm
SP 030	Length 30 mm
SP 035	Length 35 mm
SP 040	Length 40 mm
SP 045	Length 45 mm
SP 050	Length 50 mm
SP 055	Length 55 mm
SP 060	Length 60 mm
SP 065	Length 65 mm
SP 070	Length 70 mm
SP 075	Length 75 mm
SP 080	Length 80 mm
SP 085	Length 85 mm
SP 090	Length 90 mm
SP 095	Length 95 mm
SP 100	Length 100 mm



PTO Plate

Medial Opening Tibial Osteotomy Plate

ORTHOPAEDIC: The osteotomy plates (PTOD and PTOG) are used for fixation of opening wedge high tibial osteotomy and osteoarthritis of the medial tibio-femoral compartment with genu-varum.

TRAUMATOLOGY: These plates may be used for internal fixations of fractures of the medial tibial plateau.

- Parallel Epiphysal Screws
- Strengthened bridge.
- Adapted angulation and curve.
- Shapeable Plate.
- Materials:
 - > Plate: Stainless steel 316 LVM Standard ISO 5832-1 & ASTM F138&139
 - > Screws and lock-screws: Titanium TA6V Standard ISO 5832-3 & ASTM F136



References Description

PTOD	Right tibial opening plate
PTOG	Left tibial opening plate

PTO plate

Associated Surfix[®] Screws

Surfix[®] Cortical bone screw

+ lock-screw diam 4.5 mm

References Description

CC 024	Length 24 mm
CC 026	Length 26 mm
CC 028	Length 28 mm
CC 030	Length 30 mm
CC 032	Length 32 mm
CC 035	Length 35 mm
CC 040	Length 40 mm
CC 045	Length 45 mm
CC 050	Length 50 mm
CC 055	Length 55 mm
CC 060	Length 60 mm
CC 065	Length 65 mm



Surfix[®] Cancellous bone screw

+ lock-screw diam 6.5 mm

References Description

SP 020	Length 20 mm
SP 025	Length 25 mm
SP 030	Length 30 mm
SP 035	Length 35 mm
SP 040	Length 40 mm
SP 045	Length 45 mm
SP 050	Length 50 mm
SP 055	Length 55 mm
SP 060	Length 60 mm
SP 065	Length 65 mm
SP 070	Length 70 mm
SP 075	Length 75 mm
SP 080	Length 80 mm
SP 085	Length 85 mm
SP 090	Length 90 mm
SP 095	Length 95 mm
SP 100	Length 100 mm



POM Plate

Less Invasive Medial Opening Tibial Plate than PTO Plate

Fixation of opening wedge high tibial osteotomy $6^\circ < 12^\circ$.

Osteoarthritis of the medial tibiofemoral compartment with genu-varum.

- Pre-oriented screw.
- Bendable plate.
- Adapted angulation and curve.
- Strengthened bridge.
- Materials:
 - > Plate: Stainless steel 316 LVM Standard ISO 5832-1 & ASTM F138&139
 - > Screws and lock-screws: Titanium TA6V Standard ISO 5832-3 & ASTM F136



References Description

POMD	Less invasive plate for opening wedge high tibial osteotomy right side - size 1
POMG	Less invasive plate for opening wedge high tibial osteotomy left side - size 1

POM Plate

Associated Surfix® Screws

Surfix® Cortical bone screw

+ lock-screw diam 4.5 mm

References	Description
CC 024	Length 24 mm
CC 026	Length 26 mm
CC 028	Length 28 mm
CC 030	Length 30 mm
CC 032	Length 32 mm
CC 035	Length 35 mm
CC 040	Length 40 mm
CC 045	Length 45 mm
CC 050	Length 50 mm
CC 055	Length 55 mm
CC 060	Length 60 mm
CC 065	Length 65 mm



Surfix® Cancellous bone screw

+ lock-screw diam 6.5 mm

References	Description
SP 020	Length 20 mm
SP 025	Length 25 mm
SP 030	Length 30 mm
SP 035	Length 35 mm
SP 040	Length 40 mm
SP 045	Length 45 mm
SP 050	Length 50 mm
SP 055	Length 55 mm
SP 060	Length 60 mm
SP 065	Length 65 mm
SP 070	Length 70 mm
SP 075	Length 75 mm
SP 080	Length 80 mm
SP 085	Length 85 mm
SP 090	Length 90 mm
SP 095	Length 95 mm
SP 100	Length 100 mm



PTC Plate

Lateral Closing Tibial Osteotomy Plate

ORTHOPAEDICS: The osteotomy plates (PTCD and PTCG) are used for fixation of closing wedge high tibial osteotomy or for osteoarthritis of the medial tibia femoral compartment with genu-varum.

TRAUMATOLOGY: These plates may be used for internal fixations of fractures of the lateral tibial plateau.

- Pre-shaped to the tibia anatomy.
- Shapeable pegs.
- Reinforced plates.
- Materials:
 - > Plate: Stainless steel 316 LVM Standard ISO 5832-1 & ASTM F138&139
 - > Screws and lock-screws: Titanium TA6V Standard ISO 5832-3 & ASTM F136



References	Description
PTCD	Proximal tibial osteosynthesis plate right side
PTCG	Proximal tibial osteosynthesis plate left side

PTC Plate

Associated Surfix[®] Screws

Surfix[®] Cortical bone screw

+ lock-screw diam 4.5 mm

References	Description
CC 024	Length 24 mm
CC 026	Length 26 mm
CC 028	Length 28 mm
CC 030	Length 30 mm
CC 032	Length 32 mm
CC 035	Length 35 mm
CC 040	Length 40 mm
CC 045	Length 45 mm
CC 050	Length 50 mm
CC 055	Length 55 mm
CC 060	Length 60 mm
CC 065	Length 65 mm



Surfix[®] Cancellous bone screw

+ lock-screw diam 6.5 mm

References	Description
SP 020	Length 20 mm
SP 025	Length 25 mm
SP 030	Length 30 mm
SP 035	Length 35 mm
SP 040	Length 40 mm
SP 045	Length 45 mm
SP 050	Length 50 mm
SP 055	Length 55 mm
SP 060	Length 60 mm
SP 065	Length 65 mm
SP 070	Length 70 mm
SP 075	Length 75 mm
SP 080	Length 80 mm
SP 085	Length 85 mm
SP 090	Length 90 mm
SP 095	Length 95 mm
SP 100	Length 100 mm



PTF Plate

Lateral Closing Tibial Osteotomy Plate

ORTHOPAEDICS: The osteotomy plates (PTFD and PTFG) are used for fixation of closing wedge high tibial osteotomy or for osteoarthritis of the medial tibia femoral compartment with genu-varum.

TRAUMATOLOGY: These plates may be used for internal fixations of fractures of the lateral tibial plateau.

- Adapted angulation and curve to the anatomy of the tibia.
- Epiphyseal screws in the same plane.
- Adapted Angulation and Curve.
- Shapeable Plate.
- Strengthened bridge.
- Materials:
 - > Plate: Stainless steel 316 LVM Standard ISO 5832-1 & ASTM F138&139
 - > Screws and lock-screws: Titanium TA6V Standard ISO 5832-3 & ASTM F136

References	Description
PTFD	Right plate for closing wedge HTO
PTFG	Left plate for closing wedge HTO



PTF Plate

Associated Surfix® Screws

Surfix® Cortical bone screw
+ lock-screw diam 4.5 mm

References	Description
CC 024	Length 24 mm
CC 026	Length 26 mm
CC 028	Length 28 mm
CC 030	Length 30 mm
CC 032	Length 32 mm
CC 035	Length 35 mm
CC 040	Length 40 mm
CC 045	Length 45 mm
CC 050	Length 50 mm
CC 055	Length 55 mm
CC 060	Length 60 mm
CC 065	Length 65 mm



Surfix® Cancellous bone screw

+ lock-screw diam 6.5 mm

References	Description
SP 020	Length 20 mm
SP 025	Length 25 mm
SP 030	Length 30 mm
SP 035	Length 35 mm
SP 040	Length 40 mm
SP 045	Length 45 mm
SP 050	Length 50 mm
SP 055	Length 55 mm
SP 060	Length 60 mm
SP 065	Length 65 mm
SP 070	Length 70 mm
SP 075	Length 75 mm
SP 080	Length 80 mm
SP 085	Length 85 mm
SP 090	Length 90 mm
SP 095	Length 95 mm
SP 100	Length 100 mm



Osteotomy Plates ATAO[®] Bone Substitute

The substitute ATAO[®] is indicated for filling a small sized bone defects in orthopaedic surgery.

The proportion of hydroxyapatite(HA) and tricalcium phosphate(TCP) allows an optimal resorption rate compatible with the physiology of the bone cells.


References	Description
WEDo06	Bone substitute - 06°
WEDo08	Bone substitute - 08°
WEDo10	Bone substitute - 10°
WEDo12	Bone substitute - 12°
WEDo14	Bone substitute - 14°
FILo08	Granules 08 cC
FILo03	Granules 03 cC
FILo05	Granules 05 cC



*Made in France by KASIOS for Newdeal S.A.S.

Osteotomy Plates Associated Instruments

References	Description
MAo03	Surfix [®] plate bender
MAo04	Hexagonal screwdriver 3.5 mm
MAo05	Length gauge
MAo06	Drilling guide diam 3.5 mm
MAo07	Drilling guide diam 4.5 mm
MAo08	Drill AO diam 3.5 mm
MAo09	Drill AO diam 4.5 mm
MAo10	cutting closing guide
MAo38	K-wire diam 1.8 mm, L. 150 mm
MAo39	Bone substitute holder
MAo40	Trial for bone substitute
MAo41	K-wire guide diam 1.8 mm for drill guide diam 3.5 mm
MAo42	Surfix [®] distractor + 2 measurers
MAo43	Compressor
MAo47	Cutting opening guide
FPOM	Trial for POM plates
FPTOPTF	Trial plate for pto and ptf plates
FPOF	Trial for POF plates
FPTCD	Trial plate for PTCD
FPTCG	Trial plate for PTCG
SET000	Basic Tray
SET100	Osteotomy tray
SET001	Lid of osteotomy set

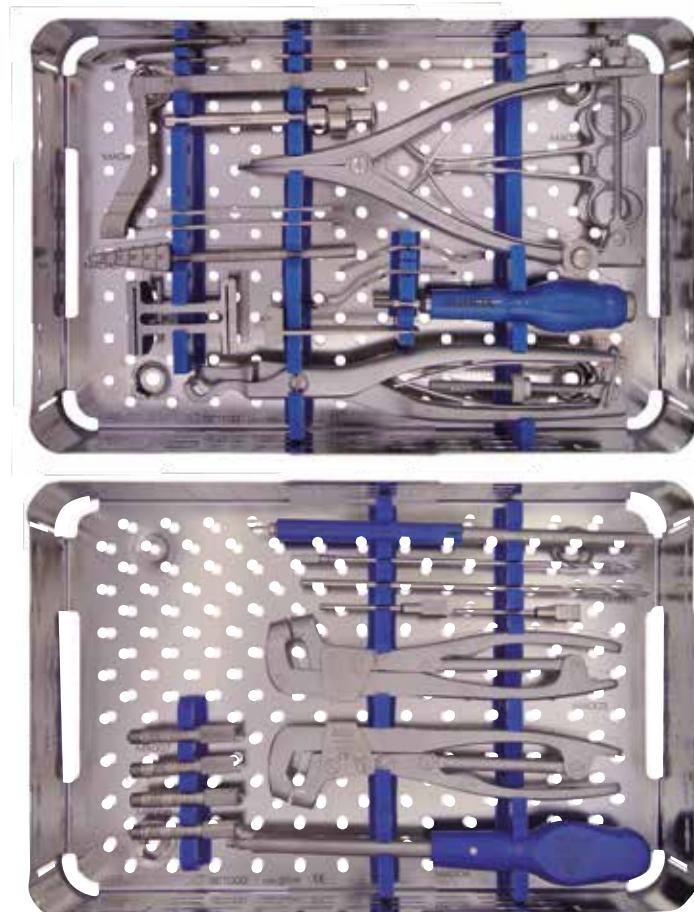

PSFE Plates

Proximal Varus and Derotation Osteotomy Plate

The osteotomy plates (PPSFE, PSFE and PPSFE D/G) are used for fixation of proximal femoral varus and derotation osteotomy for children.

- Materials:
 - > Plate: Stainless steel 316 LVM
Standard ISO 5832-1 & ASTM F138&139
 - > Screws and lock-screws: Titanium TA6V
Standard ISO 5832-3 & ASTM F136



References	Description
PPSFE	Varus osteotomy plate size 1
PSFE	Varus osteotomy plate size 2
PSFE D	Reinforced varus osteotomy plate - right side
PSFE G	Reinforced varus osteotomy plate - left side



PSFE Plates

PSFE Plates Associated Surfix® Screws

Surfix® Cortical bone screw
+ lock-screw diam 3.5 mm

References	Description
CS 016	Length 16 mm
CS 018	Length 18 mm
CS 020	Length 20 mm
CS 022	Length 22 mm
CS 024	Length 24 mm
CS 026	Length 26 mm
CS 028	Length 28 mm
CS 030	Length 30 mm
CS 032	Length 32 mm



Surfix® Cortical bone screw
+ lock-screw diam 4.5 mm

References	Description
CC 014	Length 14 mm
CC 016	Length 16 mm
CC 018	Length 18 mm
CC 020	Length 20 mm
CC 022	Length 22 mm
CC 024	Length 24 mm
CC 026	Length 26 mm
CC 028	Length 28 mm
CC 030	Length 30 mm
CC 032	Length 32 mm
CC 035	Length 35 mm
CC 040	Length 40 mm
CC 045	Length 45 mm



PSFE Plates

PSFE Associated Surfix[®] Screws

Surfix[®] Cancellous bone screw

+ lock-screw diam 6.5 mm

References	Description
SP 020	Length 20 mm
SP 025	Length 25 mm
SP 030	Length 30 mm
SP 035	Length 35 mm
SP 040	Length 40 mm
SP 045	Length 45 mm
SP 050	Length 50 mm
SP 055	Length 55 mm
SP 060	Length 60 mm



Surfix[®] Cannulated cancellous bone screw + lock-screw diam 6.5 mm

References	Description
VCA 020	Length 20 mm
VCA 025	Length 25 mm
VCA 030	Length 30 mm
VCA 035	Length 35 mm
VCA 040	Length 40 mm
VCA 045	Length 45 mm
VCA 050	Length 50 mm
VCA 055	Length 55 mm
VCA 060	Length 60 mm



PDTL Plate

Bendable Plates for Osteosynthesis

Fixation of epiphyseal, metaphyseal, diaphyseal fractures.

- Bendable plate.
- 4 sizes.
- Adapted angulation and curve.
- Materials:
 - > Plate: Stainless steel 316 LVM Standard ISO 5832-1 & ASTM F138&139
 - > Screws and lock-screws: Titanium TA6V Standard ISO 5832-3 & ASTM F136



References	Description
PD3TL52	Bendable plate 3 holes
PD4TL72	Bendable plate 4 holes
PD5TL92	Bendable plate 5 holes
PD7TL132	Bendable plate 7 holes

PDTL Reinforced Plate

Bendable and Reinforced Plates for Osteosynthesis

Fixation of epiphyseal, metaphyseal, diaphyseal fractures.

- Bendable plate.
- Reinforced bridge.
- 4 sizes.
- Adapted angulation and curve.
- Materials:
 - > Plate: Stainless steel 316 LVM Standard ISO 5832-1 & ASTM F138&139
 - > Screws and lock-screws: Titanium TA6V Standard ISO 5832-3 & ASTM F136



References	Description
PD2TL45	Bendable and reinforced plate 2 holes
PD4TL77	Bendable and reinforced plate 4 holes
PD4TL112	Bendable and reinforced plate 4 holes

PDTL Plates
Associated Surfix[®] Screws

Surfix[®] Cortical bone screw

+ lock-screw diam 3.5 mm

References	Description
CS 016	Length 16 mm
CS 018	Length 18 mm
CS 020	Length 20 mm
CS 022	Length 22 mm
CS 024	Length 24 mm
CS 026	Length 26 mm
CS 028	Length 28 mm
CS 030	Length 30 mm
CS 032	Length 32 mm



Surfix[®] Cortical bone screw

+ lock-screw diam 4.5 mm

References	Description
CC 024	Length 24 mm
CC 026	Length 26 mm
CC 028	Length 28 mm
CC 030	Length 30 mm
CC 032	Length 32 mm
CC 035	Length 35 mm
CC 040	Length 40 mm
CC 045	Length 45 mm
CC 050	Length 50 mm



Surfix[®] Cancellous bone screw


+ lock-screw diam 6.5 mm

References	Description
SP 020	Length 20 mm
SP 025	Length 25 mm
SP 030	Length 30 mm
SP 035	Length 35 mm
SP 040	Length 40 mm
SP 045	Length 45 mm
SP 050	Length 50 mm
SP 055	Length 55 mm
SP 060	Length 60 mm
SP 065	Length 65 mm
SP 070	Length 70 mm
SP 075	Length 75 mm
SP 080	Length 80 mm
SP 085	Length 85 mm
SP 090	Length 90 mm
SP 095	Length 95 mm
SP 100	Length 100 mm



Pediatric Set

Reference	Description
MA003	SURFIX® Plate bender
MA004	Hexagonal screwdriver 3.5 mm
MA005	Length gauge
MA006	Drilling guide dia. 3.5 mm
MA031	Drill guide dia. 2.7 mm
MA034	Hexagonal screwdriver 2.5 mm
MA036	Hexagonal canulated screwdriver dia. 3.5 mm
MA048	Varus Angle measurer
MA049	Ruler
MA050	Angle measurer / K-wire Guide
FPPSFE	Varus osteotomy trial plate size 1
FPSFE	Varus osteotomy trial plate size 2
FPSFED	Reinforced varus osteotomy trial plate - Right side
FPSFEG	Reinforced varus osteotomy trial plate - Left side
FPD3TL52	Bendable Trial 3 holes
FPD4TL72	Bendable Trial 4 holes
FPD5TL92	Bendable Trial 5 holes
FPD7TL132	Bendable Trial 7 holes
FPD2TL45	Bendable and reinforced trial 2 holes
FPD4TL77	Bendable and reinforced Trial 3 holes
FPD4TL112	Bendable and reinforced Trial 4 holes
MA008	Drill AO dia. 3.5 mm
MA032	Drill dia. 2.7 mm, L. 125 mm
MA037	Canulated Drill dia. 3.5 mm
MA038	K-wire dia. 1.8 mm, L. 150 mm
MA041	K-wire guide dia. 1.8 mm for drill guide dia. 3.5 mm
SET400	Tray for Pediatric
SET401	Lid for Pediatric

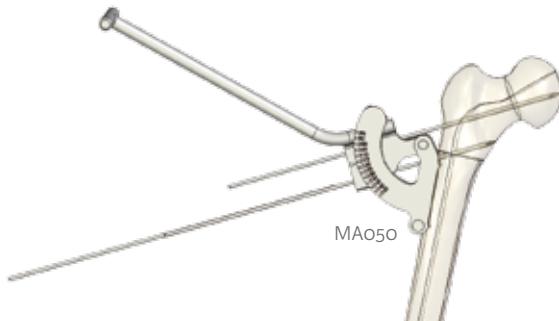



Integra® References

Index

05-0016	40	050, CC	72, 73, 74, 75, 76, 81	219 227	18
05-0017	40	050, SP	72, 73, 74, 75, 76, 79, 81	229 027 S	10
05-0106	40	050, VCA	79	229 028 S	10
05-0108	40	055, CC	72, 73, 74, 75, 76	229 037 S	10
05-0109	40	055, SP	72, 73, 74, 75, 76, 79, 81	229 038 S	10
05-0110	40	055, VCA	79	229 227 S	10
05-0112	40	060, CC	72, 73, 74, 75, 76	229 228 S	10
05-0206	40	060, SP	72, 73, 74, 75, 76, 79, 81	229 237 S	10
05-0208	40	060, VCA	79	229 238 S	10
05-0209	40	065, CC	72, 73, 74, 75, 76	295 110 S	18
05-0210	40	065, SP	72, 73, 74, 75, 76, 81	295 112 S	18
05-0212	40	070, SP	72, 73, 74, 75, 76, 81	295 114 S	18
05-1002	40	080, SP	72, 73, 74, 75, 76, 81	295 118 S	18
05-1006	40	085, SP	72, 73, 74, 75, 76, 81	295 120 S	18
05-1008	40	090, SP	72, 73, 74, 75, 76, 81	295 122 S	18
05-1009	40	095, SP	72, 73, 74, 75, 76, 81	295 124 S	18
05-1010	40	100, SP	72, 73, 74, 75, 76, 81	295 126 S	18
05-1012	40	115 008 S	10	295 128 S	18
05-1020	40	115 070	18	295 130 S	18
05-5001	40	115 070 (S)	10, 11	295 132 S	18
014, CC	78	115 100 (S)	10, 11	295 134 S	18
016, CC	78	115 116	18	299 005	18
016, CS	78, 81	119 004 (S)	11	299 020	18
018, CC	78	119 006 (S)	11	299 050	18
018, CS	78, 81	119 016 (S)	11	309 708	49
020, CC	78	119 023 (S)	10	320 100 S	18
020, CS	78, 81	119 025 (S)	10	320 200 S	18
020, SP	72, 73, 74, 75, 76, 79, 81	119 027 (S)	10	329 002	18
020, VCA	79	119 223 (S)	10	329 500	18
022, CC	78	119 225 (S)	10	329 900	18
022, CS	78, 81	119 227 (S)	10	329 901	18
024, CC	72, 73, 74, 75, 76, 78, 81	119 501	37	329 902	18
024, CS	78, 81	119 506	37	105426	36
025, SP	72, 73, 74, 75, 76, 79, 81	119 510	37	105428	36
025, VCA	79	119 516	37	105430	36
026, CC	72, 73, 74, 75, 76, 78, 81	119 522	37	105432	36
026, CS	78, 81	119 525	37	105434	36
028, CC	72, 73, 74, 75, 76, 78, 81	119 531	37	105436	36
028, CS	78, 81	119 532	37	105438	36
030, CC	72, 73, 74, 75, 76, 78, 81	119 536	37	105440	36
030, CS	78, 81	129 710	37	105445	36
030, SP	72, 73, 74, 75, 76, 79, 81	159 004 (S)	11	105450	36
030, VCA	79	159 023 (S)	10	105455	36
032, CC	72, 73, 74, 75, 76, 78, 81	159 025 (S)	10	105460	36
032, CS	78, 81	159 027 (S)	10	105640	36
035, CC	72, 73, 74, 75, 76, 78, 81	159 223 (S)	10	105645	36
035, SP	72, 73, 74, 75, 76, 79, 81	159 225 (S)	10	105650	36
035, VCA	79	159 227 (S)	10	105655	36
040, CC	72, 73, 74, 75, 76, 78, 81	189 210	18	105660	36
040, SP	72, 73, 74, 75, 76, 79, 81	189 215	18	105665	36
040, VCA	79	189 220	18	105670	36
045, CC	72, 73, 74, 75, 76, 78, 81	195 100 S	18	105675	36
045, SP	72, 73, 74, 75, 76, 79, 81	219 027	18	105680	36
045, VCA	79	219 127	18	105685	36

105690	36	111765S	35	117255	24
111010	14	111770S	35	117260	24
111012	14	111775S	35	117340	24
111014	14	111780S	35	117345	24
111016	14	111785S	35	117350	24
111018	14	111790S	35	117440	24
111020	14	111795S	35	117445	24
111022	14	111800S	35	117450	24
111024	14	111805S	35	119050	17, 66
111026	14	111810S	35	119104	34
111028	14	111815S	35	119105	10
111312	14	111820S	35	119106	17, 66, 67
111314	14	112011	15, 16	119133	27
111316	14	112012	15, 16	119135	27
111318	14	112013	15, 16	119138	34
111320	14	112014	15, 16	119139	34
111322	14	112111	15	119150	35
111324	14	112111S	15	119151	35
111326	14	112112	15	119152	35
111328	14	112112S	15	119153	35
111328S	26	112113	15	119154	35
111330	14	112113S	15	119155	35
111330S	26	112114(S)	15	119156	35
111332	14	112114S	15	119170	35
111332S	26	114438	34	119171	35
111334	14	115070	27	119172	35
111334S	26	115100	25, 27, 42	119173	35
111424	34	115101	43	119174	35
111426	34	115116	27, 34, 38, 47, 63	119175	35
111428	34	115216	21, 25, 28, 60	119176	35
111430	34	115225	37, 38, 47, 63	119177	35
111432	34	115425	60	119311	11
111434	34	115516	35	119510	37
111436	34	117010	25	119516	34
111440	34	117012	25	119531	38
111445	34	117014	25	119541	37
111450	34	117016	25	119546	37
111455	34	117018	25	119551	37
111460	34	117020	25	119552	37, 58
111530S	35	117022	25	119555	37
111535S	35	117024	25	119561	37, 38
111540S	35	117026	25	119562	37
111545S	35	117028	25	119566	37
111550S	35	117030	25	119580	38
111555S	35	117032	25	119582	38
111560S	35	117034	25	119590	38
111565S	35	117110	25	119592	38
111570S	35	117112	25	119601	21
111575S	35	117114	25	119609	47
111580S	35	117116	25	119611	21, 47
111740S	35	117118	25	119618	25
111745S	35	117150	24	119631	49
111750S	35	117155	24	119632	49
111755S	35	117160	24	119641	47
111760S	35	117250	24	119645	21

250
240
230
220
210
200
190
180
170
160
150
140
130
120
110
100
90
80
70
60
50
40
30
20
10
0

MILLIMETERS

119646.....	47	119863.....	39	121815S	35
119647.....	47	119864.....	39	121820S.....	35
119651.....	65, 67	119865.....	39	121950.....	35
119653.....	65, 67	119867.....	39	121951.....	35
119654.....	65, 67	119880.....	39	129710.....	25, 27, 28, 37
119657.....	49	119881.....	39	129714.....	25, 27, 28
119659.....	49	119882.....	39	129716.....	25, 27, 28
119662.....	47	119909, 19, 21, 25, 27, 29, 35, 37, 42, 43, 47, 56, 58, 60, 63, 67		129718.....	25, 27, 28
119664.....	47, 65	119935.....	34	129720.....	25, 27, 28
119665.....	47	119936.....	34	129722.....	27, 28
119666.....	47	119937.....	34	129724.....	25, 27, 28
119667.....	47	119938.....	34	129726.....	25, 27, 28
119669.....	47	119949.....	37	129728.....	25, 27, 28
119690.....	47	119951.....	37	129730.....	25, 27, 28
119691.....	47	119953.....	37	129731.....	25
119692.....	47	119955.....	38	129732.....	25
119693.....	47	119956.....	37	129733.....	25
119694.....	47	119957.....	37	129734.....	25
119695.....	47	119958.....	37	129735.....	25
119696.....	47	119959.....	38	129736.....	25
119697.....	47	119965.....	49	129752.....	27, 28
119698.....	47	119966.....	49	129930.....	25
119699.....	47	119967.....	49	129931.....	25
119700.....	64	119974.....	37	129932.....	25
119751.....	47	119975.....	38	129933.....	25
119757.....	49	119976.....	37	129935.....	28
119760.....	49	119977.....	38	129936.....	25
119761.....	49	119978.....	49	129938.....	28
119762.....	49	119989.....	67	131014S.....	14
119763.....	49	121530S.....	35	131016S.....	14
119764.....	49	121535S.....	35	131018S.....	14
119765.....	49	121540S.....	35	131020S.....	14
119766.....	49	121545S.....	35	131022S.....	14
119767.....	49	121550S.....	35	131024S.....	14
119768.....	49	121555S.....	35	131026S.....	14
119769.....	49	121560S.....	35	131028S.....	14
119778.....	47	121565S.....	35	131030S.....	14
119779.....	47	121570S.....	35	131032S.....	14
119790.....	49	121575S.....	35	131034S.....	14
119791.....	49	121580S.....	35	139100–106.....	21
119792.....	49	121740S.....	35	139107.....	21
119793.....	49	121745S.....	35	139111–116.....	21
119794.....	49	121750S.....	35	139120.....	21
119795.....	49	121755S.....	35	139121.....	21
119796.....	49	121760S.....	35	139121–126.....	21
119797.....	49	121765S.....	35	139128.....	21
119798.....	49	121770S.....	35	139129.....	21
119799.....	49	121775S.....	35	139140.....	21
119825.....	39	121780S.....	35	139150.....	21
119831.....	39	121785S.....	35	139201–205.....	21
119850.....	39	121790S.....	35	139210.....	21
119859.....	39	121795S.....	35	139211.....	21
119860.....	39	121800S.....	35	139211–215.....	21
119861.....	39	121805S.....	35	139216.....	21
119862.....	39	121810S.....	35	139311–313.....	21

139321–323	21	159960	63	200022S	14
139331–333	21	159991	63	200024S	14
139341–343	21	169001	60	200026S	14
139351–353	21	169002	60	200028S	14
139940	21	169003	60	200030S	14
139941	21	169004	60	201010	22
139942	21	169021	42	201020	22
139943	21	169022	42	201030	22
139953	21	169023	42	201040	22
141009	39	169031	42	202010	22
141010	39	169032	42	202020	22
141011	39	169033	42	202030	22
141012	39	169041	42	202040	22
141013	39	169042	42	203010	22
141014	39	169051	42	203020	22
141015	39	169052	42	203030	22
141017	39	169101	60	203040	22
150010S	61	169102	42	203100	22
150020S	61	169104	60	203200	22
150030S	61	169105	60	203300	22
150040S	61	169106	42, 43	203415	22
150110S	61	169107	42	203500	22
150120S	61	169111	60	203600	22
150130S	61	169112	42	205000	22
150200S	62	181001S	59	213113	16
150240S	62	181002S	59	213114	16
150242S	62	181003S	59	213115	16
150246S	62	181004S	59	213116	16
150250S	62	181011S	59	213117	16
150255S	62	181012S	59	213213	16
150260S	62	181013S	59	213214	16
150265S	62	181014S	59	213215	16
150270S	62	181021S	41	213216	16
150275S	62	181022S	41	213217	16
150280S	62	181023S	41	213313	16
150285S	62	181031S	41	213314	16
150290S	62	181032S	41	213315	16
150514S	61	181033S	41	213316	16
150516S	61	181041S	41	213317	16
159010	63	181042S	41	213512	16
159020	63	181051S	41	213820	16
159027S	27	181052S	41	219027	27
159071	63	185100S	26	219035	63
159103	63	185200S	26	219127	27
159106	63	185300S	41, 43, 62	219135	63
159109	63	185400S	59	219227	27
159110	63	185600S	59	219335	42, 43, 63
159120	63	195100S	26	219345	60
159127	47	195200S	26	219365	60
159130	63	200010(S)	14	219435	42, 43, 63
159400	63	200012S	14	219445	60, 63
159635	63	200014S	14	219465	60
159740	63	200016S	14	219535	42, 43, 63
159755	63	200018S	14	219545	60, 63
159760	63	200020S	14	219565	60

250

240

230

220

210

200

190

180

170

160

150

140

130

120

110

100

90

80

50

40

30

20

10

MILLIMETERS

219627	27	250311	20	285322S	41, 43, 62
219635	42, 43, 63	250312	20	285324S	41, 43, 62
219645	60	250321	20	285326S	41, 43, 62
219665	60	250322	20	285328S	41, 43, 62
219735	42, 43	250323	20	285330S	41, 43
219765	60	250331	20	285330S	62
219835	42, 43, 63	250332	20	285332S	41, 43, 62
219845	60, 63	250333	20	285334S	41, 43, 62
219865	60	250341	20	285336S	43
219900	60	250342	20	285336S	62
219960	63	250343	20	285338S	43
229002	10	250351	20	285338S	62
229003	10	250352	20	285340S	43
229004	10	250353	20	285340S	62
229005	10	275560	47	285344S	62
229011	10, 17, 66	278002S	29	285348S	62
229012	10, 17, 66	278005S	29	285350S	62
229101	10, 11	278007S	29	285414S	59
229102	11	278008S	29	285416S	59
229201	11	278009S	29	285418S	59
229202	11	278010S	29	285420S	59
229951	10	278100	29	285422S	59
229952	11	278110	29	285424S	59
229961	10	278119	29	285426S	59
229962	11	278121	29	285428S	59
229965	12	278122	29	285430S	59
229966	13	278123	29	285435S	59
229970	8, 10, 11	278124	29	285440S	59
229971	10	278900	29	285445S	59
229975	12	278901	29	285450S	59
229976	13	278902	19, 29	285455S	59
229990	8	285110S	26	285460S	59
229996	8	285112S	26	285465S	59
230001S	19	285114S	26	285625S	59
230002S	19	285116S	26	285630S	59
239000	19	285118S	26	285635S	59
239001	19	285120S	26	285640S	59
239011	19	285122S	26	285645S	59
239012	19	285124S	26	285650S	59
239021	19	285126S	26	285655S	59
239022	19	285210S	26	285660S	59
239030	19	285212S	26	285665S	59
239500	19	285214S	26	290150S	26
250100	20	285216S	26	290155S	26
250101	20	285218S	26	290160S	26
250102S	20	285220S	26	290250S	26
250103	20	285222S	26	290255S	26
250104	20	285224S	26	290260S	26
250105	20	285226S	26	290340S	26
250106	20	285310S	41, 62	290345S	26
250201	20	285312S	41, 43, 62	290350S	26
250202	20	285314S	41, 43, 62	290440S	26
250203	20	285316S	41, 43, 62	290445S	26
250204	20	285318S	41, 43, 62	290450S	26
250205	20	285320S	41, 43, 62	295110S	26

295112S.....	26	299900.....	27	301233.....	48
295114S.....	26	299901.....	27	301234.....	48
295116S.....	26	299903.....	27	301235.....	48
295118S.....	26	299904.....	27	302110.....	45
295120S.....	26	300005.....	45	302111.....	45
295122S.....	26	300006.....	45	302112.....	45
295124S.....	26	300007.....	45	302113.....	45
295126S.....	26	300009.....	45	302114.....	45
295210S.....	26	300105.....	45	302115.....	45
295212S.....	26	300106.....	45	302116.....	45
295214S.....	26	300107.....	45	302121.....	48
295216S.....	26	300109.....	45	302122.....	48
295218S.....	26	300205.....	45	302123.....	48
295220S.....	26	300206.....	45	302124.....	48
295222S.....	26	300207.....	45	302125.....	48
295224S.....	26	300209.....	45	302201.....	44
295226S.....	26	300305.....	45	302202.....	44
295310S.....	62	300306.....	45	302203.....	44
295310S.....	62	300307.....	45	302204.....	44
295312S.....	62	300309.....	45	302205.....	44
295314S.....	62	300405.....	45	302206.....	44
295316S.....	62	300406.....	45	302222.....	48
295318S.....	62	300407.....	45	302223.....	48
295320S.....	62	300409.....	45	302224.....	48
295322S.....	62	300505.....	45	302225.....	48
295324S.....	62	300506.....	45	302232.....	48
295326S.....	62	300507.....	45	302233.....	48
295328S.....	62	300509.....	45	302234.....	48
295330S.....	62	300605.....	45	302235.....	48
295332S.....	62	300606.....	45	303312S.....	48
295334S.....	62	300607.....	45	303316S.....	48
295336S.....	62	300609.....	45	303320S.....	48
295338S.....	62	301110.....	45	303328S.....	45
295340S.....	62	301111.....	45	303330S.....	45
295344S.....	62	301112.....	45	303334S.....	45, 48
295348S.....	62	301113.....	45	303338S.....	45, 48
295350S.....	62	301114.....	45	303340S.....	45, 48
299005.....	27	301115.....	45	303342S.....	45, 48
299010.....	27	301116.....	45	303512S.....	53
299020.....	27	301121.....	48	303516S.....	53
299050.....	27	301122.....	48	303520S.....	53
299070.....	27	301123.....	48	303530S.....	51
299080.....	27	301124.....	48	303534S.....	51, 53
299150.....	27	301125.....	48	303538S.....	51, 53
299155.....	27	301201.....	44	303540S.....	51, 53
299160.....	27	301202.....	44	303542S.....	51, 53
299250.....	27	301203.....	44	309200.....	47
299255.....	27	301204.....	44	309300.....	47
299260.....	27	301205.....	44	309301.....	47
299340.....	27	301206.....	44	309302.....	47
299345.....	27	301222.....	48	309303.....	47
299350.....	27	301223.....	48	309304.....	47
299440.....	27	301224.....	48	309305.....	47
299445.....	27	301225.....	48	309306.....	47
299450.....	27	301232.....	48	309309.....	47

309360.....	47	309773.....	47	352254.....	50
309361.....	47	309900.....	47	352255.....	50
309362.....	47	309902.....	47	352256.....	50
309363.....	47	309904.....	47	352512.....	53
309364.....	47	309920.....	47	352513.....	53
309365.....	47	309940.....	47	352514.....	53
309366.....	47	309942.....	47	352515.....	53
309370.....	47	309960.....	47	352522.....	52
309371.....	47	309970.....	47	352523.....	52
309372.....	47	309980.....	47	352524.....	52
309373.....	47	330021S.....	43	352525.....	52
309374.....	47	330023S.....	43	352532.....	52
309375.....	47	330025S.....	43	352533.....	52
309376.....	47	330217S.....	43	352534.....	52
309601.....	47	330220S.....	43	352535.....	52
309604.....	47	330225S.....	43	500001.....	54
309605.....	47	330230S.....	43	500050.....	54
309606.....	47	330420S.....	43	500080.....	54
309607.....	47	330425S.....	43	500150.....	54
309608.....	47	330430S.....	43	500180.....	54
309615.....	47	339001.....	43	500250.....	54
309620.....	47	339003.....	43	500280.....	54
309622.....	47	339004.....	43	500350.....	54
309623.....	47	339005.....	43	500380.....	54
309624.....	47	339920.....	43	501020.....	55
309625.....	47	339950.....	43	501022.....	55
309626.....	47	351152.....	51	501025.....	55
309627.....	47	351153.....	51	501027.....	55
309630.....	47	351154.....	51	501030.....	55
309635.....	47	351155.....	51	501035.....	55
309636.....	47	351251.....	50	501040.....	55
309637.....	47	351252.....	50	501045.....	55
309645.....	47, 58	351253.....	50	501050.....	55
309652.....	47	351254.....	50	501055.....	55
309656.....	47	351255.....	50	501060.....	55
309657.....	47	351256.....	50	501065.....	55
309661.....	47	351512.....	53	501070.....	55
309680.....	47	351513.....	53	501075.....	55
309681.....	47	351514.....	53	501080.....	55
309682.....	47	351515.....	53	501085.....	55
309683.....	47	351522.....	52	501090.....	55
309684.....	47	351523.....	52	501095.....	55
309685.....	47	351524.....	52	501100.....	55
309686.....	47	351525.....	52	501105.....	55
309690.....	47	351532.....	52	501110.....	55
309691.....	47	351533.....	52	510005.....	54
309692.....	47	351534.....	52	510111.....	54
309693.....	47	351535.....	52	510141.....	54
309694.....	47	352152.....	51	510211.....	54
309695.....	47	352153.....	51	510241.....	54
309696.....	47	352154.....	51	510311.....	54
309697.....	47	352155.....	51	510341.....	54
309699.....	47	352251.....	50	511020.....	55
309712.....	49	352252.....	50	511022.....	55
309753.....	47	352253.....	50	511025.....	55

511027.....	55	519184.....	56	998030.....	67
511030.....	55	519185.....	56	998031.....	67
511035.....	55	519209.....	58	999001.....	30, 68
511040.....	55	519210.....	58	999002.....	30, 68
511045.....	55	519290.....	56	999003.....	30, 68
511055.....	55	519295.....	56	999004.....	30, 68
511060.....	55	519910.....	56	999100.....	30, 68
511065.....	55	519911.....	56	999101.....	30, 68
511070.....	55	519912.....	56	999102.....	30, 68
511075.....	55	519920.....	56		
511080.....	55	519950.....	58		
511085.....	55	519951.....	58		
511090.....	55	529061.....	35	Advansys™ Dorsal Lisfranc Plates.....	41
511095.....	55	539015.....	56	Advansys™ Medial Lisfranc Plate.....	41
511100.....	55	539020.....	56	Advansys™ TTC Fusion Plate.....	59
511105.....	55	539021.....	56	ALG-890-00.....	23
511110.....	55	539022.....	56	ATAO® Bone Graft Substitute.....	77
519002.....	56	539023.....	56		
519003.....	56	996100.....	19, 28, 29, 58		
519004.....	56	996200.....	18, 25, 27, 35, 37, 42, 43, 60, 63		
519005.....	56	996350.....	47	C	
519006.....	56	996400.....	34	CC 024.....	72, 73, 74, 75, 76, 81
519007.....	56	997034.....	47	CC 026.....	72, 73, 74, 75, 76, 81
519008.....	56	997035.....	47	CC 028.....	72, 73, 74, 75, 76, 81
519009.....	56	997100.....	27	CC 030.....	72, 73, 74, 75, 76, 81
519010.....	56	997301.....	10, 11	CC 032.....	72, 73, 74, 75, 76, 81
519011.....	56	997311.....	10	CC 035.....	72, 73, 74, 75, 76, 81
519012.....	56	998001.....	67	CC 040.....	72, 73, 74, 75, 76, 81
519013.....	56	998002.....	67	CC 045.....	72, 73, 74, 75, 76, 81
519014.....	56	998003.....	67	CC 050.....	72, 73, 74, 75, 76, 81
519015.....	56	998004.....	67	CC 055.....	72, 73, 74, 75, 76
519016.....	56	998005.....	67	CC 060.....	72, 73, 74, 75, 76
519017.....	56	998006.....	67	CC 065.....	72, 73, 74, 75, 76
519020.....	56	998007.....	67	CS 016.....	81
519021.....	56	998008.....	67	CS 018.....	81
519028.....	56	998010.....	67	CS 020.....	81
519029.....	56	998011.....	67	CS 022.....	81
519030.....	56	998012.....	67	CS 024.....	81
519032.....	56	998013.....	67	CS 026.....	81
519034.....	56	998014.....	67	CS 028.....	81
519040.....	56	998015.....	67	CS 030.....	81
519110.....	56	998016.....	67	CS 032.....	81
519120.....	56	998017.....	67		
519121.....	56	998018.....	67	D	
519130.....	56	998019.....	67	DCG-890-00.....	23
519131.....	56	998020.....	67	DRL-890-00.....	23
519133.....	56	998021.....	67		
519135.....	56	998022.....	67	F	
519160.....	56	998023.....	67	FIL003.....	77
519175.....	56	998024.....	67	FIL005.....	77
519178.....	56	998025.....	67	FIL008.....	77
519179.....	56	998026.....	67	FPD2TL45.....	82
519180.....	56	998027.....	67	FPD3TL52.....	82
519181.....	56	998028.....	67	FPD4TL72.....	82
519183.....	56	998029.....	67		

TRL-890-40PPT 23

U

UNI-CP™ 43

W

WED006 77
WED008 77
WED010 77
WED012 77
WED014 77

250
240
230
220
210
200
190
180
170
160
150
140
130
120
110
100
90
80
70
60
50
40
30
20
10
MILLIMETERS



Distributed by

Integra LifeSciences Services (France) SAS

Sales & Marketing EMEA

Immeuble Séquoia 2 ■ 97 allée Alexandre Borodine

Parc technologique de la Porte des Alpes

69800 Saint Priest ■ FRANCE

Phone: +33 (0)4 37 47 59 00 ■ Fax: +33 (0)4 37 47 59 99

emea.info@integralife.com ■ integralife.eu

Customer Services

International: +33 (0)4 37 47 59 50 ■ +33 (0)4 37 47 59 25 (Fax) ■ csemea@integralife.com

United Kingdom: +44 (0)1 264 345 781 ■ +44 (0)1 264 363 782 (Fax) ■ csuk.ortho@integralife.com

France: +33 (0)4 37 47 59 10 ■ +33 (0)4 37 47 59 29 (Fax) ■ cs-ortho@integralife.com

Benelux: +32 (0)2 257 4130 ■ +32 (0)2 253 2466 (Fax) ■ custsvcbenelux@integralife.com

Switzerland: +41 (0)2 27 21 23 30 ■ +41 (0)2 27 21 23 99 (Fax) ■ custsvcsuisse@integralife.com

©2013 Integra LifeSciences Corporation. All rights reserved. ILS 02-02-004-01-12 / ILS 02-02-006-01-12 / ILS 08-02-009-02-12

PRODUCTS FOR SALE IN EUROPE, MIDDLE-EAST and AFRICA ONLY



Availability of these products might vary from a given country or region to another, as a result of specific local regulatory approval or clearance requirements for sale in such country or region. Always refer to the appropriate instructions for use for complete clinical instructions. Non contractual document. The manufacturer reserves the right, without prior notice, to modify the products in order to improve their quality. WARNING: Applicable laws restrict these products to sale by or on the order of a physician. All text and diagrams contained in this catalog are intended as guidelines and are for illustrative purposes only. No information included in this catalog is intended to replace the Directions for Use packaged with each Integra product. Always refer to the appropriate Directions for Use for complete clinical instructions. For technical and additional clinical information on Integra products, please contact your Integra local sales representative. Prado is a registered trademark of its owner. MBA, Uni-CP and K2 are trademarks of Integra Lifesciences Corporation or its subsidiaries. I.C.O.S., Traumax, ATO, Kalix, Advansys, Hintergra, Panta, Tibaxys, Achillion, Hintermann, Solustaple, K-Fix, B-Bop, Ipp-On, Metis, Hallu, Qwix, Bold, Uni-Clip, Spin, Snap-Off, Wifix, Surfix, Integra and the Integra logo are registered trademarks of Integra Lifesciences Corporation or its subsidiaries in the United States and/or other countries. All the references numbers mentioned on this document are CE marked according to European council directive 93/42/EEC on medical devices and its relatives, unless specifically identified as "NOT CE MARKED."